




Product catalog
CONOLOG[®] Implant System

Valid from August 2020

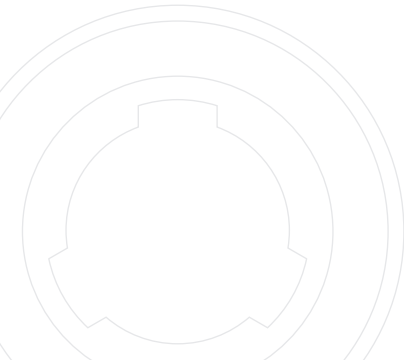

Content

System information

The CONELOG® Implant System	2
-----------------------------	---

Surgery

Planning	16
PROGRESSIVE-LINE Implants and instruments	19
PROGRESSIVE-LINE Flex instruments	24
PROGRESSIVE-LINE Guide System	28
SCREW-LINE Implants and instruments	33
SCREW-LINE Guide System Implants and instruments	38
General surgical instruments	42
Osteotomy set	49
ALTApin set	53
Cover screws	55
Healing caps	55

Prosthetics

Impression taking	58
Bite registration	59
Fabrication of the plaster model	59
Temporary restoration	60
Esthomic® Abutments	60
CAD/CAM prosthetics	62
CAM titanium blanks	64
Universal abutments	65
Gold-plastic abutment	65
Logfit® Prosthetic system	66
COMFOUR® System	67
Ball abutment anchoring system	71
Locator® Anchoring system	72
Double crown restorations	77
Accessories for abutments	77
Prosthetic instruments	78
Instruments for dental technicians	82
Selection abutments	83

Auxiliary article

Implants for practice	86
Demonstration models	87
Macro models	87
Literature	88

Auxiliary information

Indication overview	90
Implant overview	93
Prosthetics overview	94
Screw overview	100
Overview tightening torque	104
Materials	106

Index

Alphabetical	108
Article number	112
Further documentation	122

The CONELOG® Implant System



The CONELOG® Implant System is based on years of clinical and laboratory experience and is a user-friendly, consistent prosthetically oriented implant system.

All CONELOG® Products are manufactured with the latest state-of-the-art technology. The CONELOG® Implant System is continuously being developed by the company's research and development team in collaboration with clinics, universities and dental technicians and therefore stays abreast of the latest technology.

The CAMLOG® and CONELOG® Implant Systems are very well documented scientifically. Studies* support this with respect to a great many parameters including the implant surface, time of implantation and/or implant loading, primary stability, and the connection design. The long-term results of the Promote® Surface are convincing.

The descriptions that follow are not adequate to permit immediate use of the CONELOG® Implant System.

Instruction by a surgeon experienced in using the system is strongly recommended. CONELOG® Products should only be used by dentists, doctors, surgeons and dental technicians who have been trained in using the system. Appropriate courses and training sessions are regularly offered by Camlog.

Methodological errors in treatment can result in loss of the implant and significant loss of peri-implant bone.

Not all products and services from Camlog are available in all countries.

Packaging units: unless described otherwise, each pack contains one product.

The images in this document are for reference purposes only and may differ from the actual product.

* See «Further documentation» on page 122

CONELOG® PROGRESSIVE-LINE Implants

The new CONELOG® PROGRESSIVE-LINE Implants make it easier to implement modern treatment concepts such as immediate restorations or immediate loading, which require high primary stability [1, 2]*.

The geometry of the implant is consistently designed to develop high initial stability:

- The self-tapping screw implant has a conically shaped apical area that enables pronounced primary stability even in soft bone [1, 2]*.
- Thread extending to the apex for good anchorage in immediate implantations [1, 2]*.
- Crestal thread for improved hold with limited bone height [2]*.

CONELOG® PROGRESSIVE-LINE Implants are available with the abrasive-blasted, acid-etched Promote® Surface which extends over the entire implant body up to the acid-etched conical 45° implant shoulder. Depending on the clinical situation, this surface design thus permits epicrestal or slightly subcrestal implant positioning in the sense of a classic bone level implant.

PROGRESSIVE-LINE Implants with screw-mounted insertion post can be used for the guided implantation.


CONELOG® PROGRESSIVE-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.



CONELOG® PROGRESSIVE-LINE
Implant Promote® plus

* see «Further documentation» on page 122.

Implant diameters



3.3 mm 3.8 mm 4.3 mm 5.0 mm

Implant lengths



7 mm 9 mm 11 mm 13 mm 16 mm



CONELOG® SCREW-LINE
Implant Promote® plus

CONELOG® SCREW-LINE Implants


CONELOG® SCREW-LINE Implants are slightly conical, self-tapping screw implants. They enable easy insertion by self-centering with continuous bone contact to achieve solid primary stability.

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® surface up to the acid-etched conical 45° implant shoulder and thus allow for maximum flexibility when determining the vertical implant position. Rounding of the apical geometry ensures gentle insertion of the CONELOG® SCREW-LINE Implants into the bone, also near the maxillary sinus.

SCREW-LINE Implants with screw-mounted insertion post can be used for the guided implantation.

CONELOG® SCREW-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.

Implant diameters



3.3 mm 3.8 mm 4.3 mm 5.0 mm

Implant lengths



7 mm 9 mm 11 mm 13 mm 16 mm

All CONELOG® Implants are delivered pre-assembled in sterile packaging on a color-coded insertion post corresponding to the diameter.

CONELOG® Implant-Abutment connection


The geometry of the CONELOG® Implant-Abutment connection enables integrated Platform Switching and provides excellent tactile feedback when inserting the abutments. Indexing via the three grooves/cams allows the cams to slide noticeably into the grooves of the implant and thus into the final position when the abutment is rotated slightly. Simple, easy and safe orientation in the longitudinal axis of the implant is thus ensured. The precise conical connection minimizes micro-movements and demonstrates superior stability compared to other conical connections [3, 4]*.

* See „Further documentation“ on page 122

Advantages and benefits of the CONELOG® Connection

- Simple, fast and precise abutment positioning with clearly noticeable tactile feedback
- Precise, conical implant-abutment connection with superior stability compared to other conical connections
- Integrated Platform Switching

For optimal positioning of the abutments, the implant should be aligned in the bone so that one of the three grooves points in vestibular direction. With the CONELOG® Implants, the insertion tools include markings that correspond to the three grooves of the implant inner configuration.

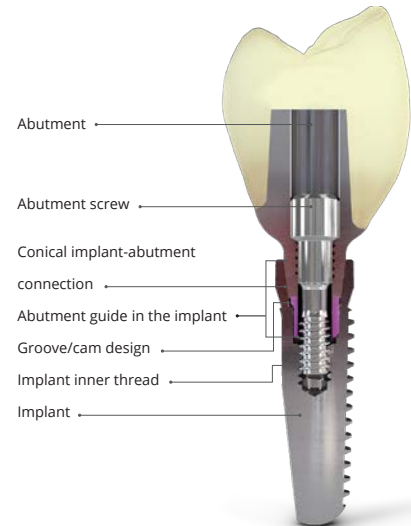

Promote® Surface

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® Surface. The surface is based on current scientific knowledge and supports rapid osseointegration. Scientific results from studies with cell cultures, osteohistology and in pull-out trials illustrate this impressively.



Production precision

The inner and outer geometry of the CONELOG® Implants and abutments are rotary machined for the most part. The tolerances can therefore be kept very low. The result is excellent part precision without impacting the material structure. The CONELOG® Implant-abutment connection thus ensures a very precise, stable and rotation-locked connection to the prosthetic components.

CONELOG® Prosthetic components

The CONELOG® SCREW-LINE Implants can be provided with a wide range of flexible, anatomically adapted prosthetic components. CONELOG® Abutments are color-coded according to the implant diameters.

Effect of the Platform Switching design

The CONELOG® Implant system offers integrated Platform Switching as the implant shoulder is not covered by the healing caps and abutments. Platform Switching option is used to support the hard and soft tissue in the peri-implant esthetic region. The distance between the implant-abutment interface and the alveolar crest is increased and thereby reduces the effect of inflammatory cell infiltration with concomitant bone resorption.



CONELOG® Healing caps

CONELOG® Healing caps sit on the machined implant shoulder, but do not cover it completely. As a result, the soft tissue over the shoulder can be adapted. The conical surfaces do not come into contact.

The healing caps are used according to indication for single and two-stage procedures. The healing caps are available in three geometries (cylindrical, wide body and bottleneck) and are screwed directly into the implant.

CONELOG® Impression taking

Impression-taking of the CONELOG® Implants is possible with impression posts, open or closed tray. All impression-taking components are color-coded based on the implant diameter. High-precision components ensure correct transfer of the intraoral situation.

The CONELOG® Impression posts do not lock into the cone of the implant, but lie on the implant shoulder. Thus, a vertical offset is prevented when taking the impression. The antirotational mechanism is ensured by the CONELOG® Groove/cam geometry.





CONELOG® Temporary abutments

CONELOG® Temporary abutments made of titanium alloy are available for temporary restorations in crown and bridge versions. The abutments can be used in immediate implantations or after exposing the gingiva.

CONELOG® Titanium bases CAD/CAM

CONELOG® Titanium bases CAD/CAM are acting as a bonding basis for customized, implant-supported dental restorations made of suitable materials. Reconstructions are fabricated with the aid of CAD/CAM techniques. CONELOG® Titanium bases CAD/CAM are available in crown and bridge versions in the gingival heights 0.8 and 2.0 mm.




CONELOG® Esthomic® Abutments

Anatomically preformed abutments allow for optimal stump design. The CONELOG® Esthomic® Abutments are available both straight and angled with various gingival heights and with an oval anatomically pre-shaped shoulder profile. The angled Esthomic® Abutments are available in A and B versions differentiated by a cam offset of 60°. This results in six prosthetic-oriented rotating positions and allows perfect prosthetic alignment of the axes.



CONELOG® Esthomic® Abutment cam alignment

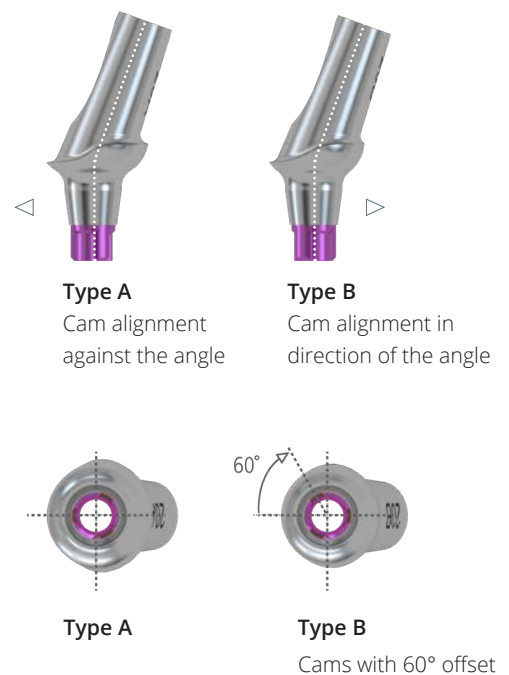

CONELOG® Gold-plastic abutment

The CONELOG® Gold-plastic abutment can be used with the cast-on technique to fabricate a multitude of customized implant restorations, such as single crowns, mesostructures for cementable bridge restorations and primary abutments for bridging implant axis divergences in the double crown technique.



CONELOG® Logfit® Abutments

The CONELOG® Logfit® Prosthetic System can be used for fabricating cementable crown and bridge restorations. The Logfit® Prosthetic System consists of prefabricated components precisely matched to one another and thus standardizes the clinical and technical procedure. The result is a lower workload for the practice and the dental laboratory.



CONELOG® Universal and telescope abutment

CONELOG® Universal and telescope abutments can be used for individually fabricated cementable crown and bridge restorations and for double crown restorations. The abutments are made of titanium alloy and can be custom trimmed.



CONELOG® Ball, Locator® and straight bar abutments

Ball, Locator® and straight bar abutments are available for the CONELOG® Implant System. These differ from the abutments in the apical region through different connection designs. Ball, Locator® and straight bar abutments are manufactured as single pieces with a thread in the apical region which engages with the inner thread of the CONELOG® Implant. These abutments are screwed into the CONELOG® Implant using the corresponding insertion tools.



Example: CONELOG® Ball abutment (Ø 4.3 m)
in a CONELOG® SCREW-LINE Implant

CONELOG® Disconnecter for CONELOG® Abutments


A special CONELOG® Disconnecter is available for the easy removal of CONELOG® Abutments from CONELOG® Implants or lab analogs. First the CONELOG® Abutment screw/ or lab screw is removed and the disconnecter is screwed into the screw canal until the abutment releases from the internal cone of the CONELOG® Implant or lab implant.



COMFOUR® System

Occlusally screw-retained restorations are state-of-the-art. With the COMFOUR® System, edentulous patients are given the option of immediate, comfortable and permanent dentures on four or six implants as a rule – and thus a considerable gain in quality of life. But clinicians too can look forward to considerably greater comfort and freedom. COMFOUR® offers several treatment concepts. In addition to occlusally screw-retained crowns and bridges for immediate and delayed restorations, the multi-optional system also permits bar restorations on straight and angled bar abutments.

COMFOUR® offers a wide range of options to master the challenges in practice routine easier and with less time in future. Next to its versatility, the COMFOUR® Prosthetic system excels through its slim design in particular. All components are of delicate and low design, which simplifies prosthetic restorations considerably for dentists and dental technicians. In addition, a number of technical highlights ensure that COMFOUR® is not simply just a name, but also a program – for users and patients alike.

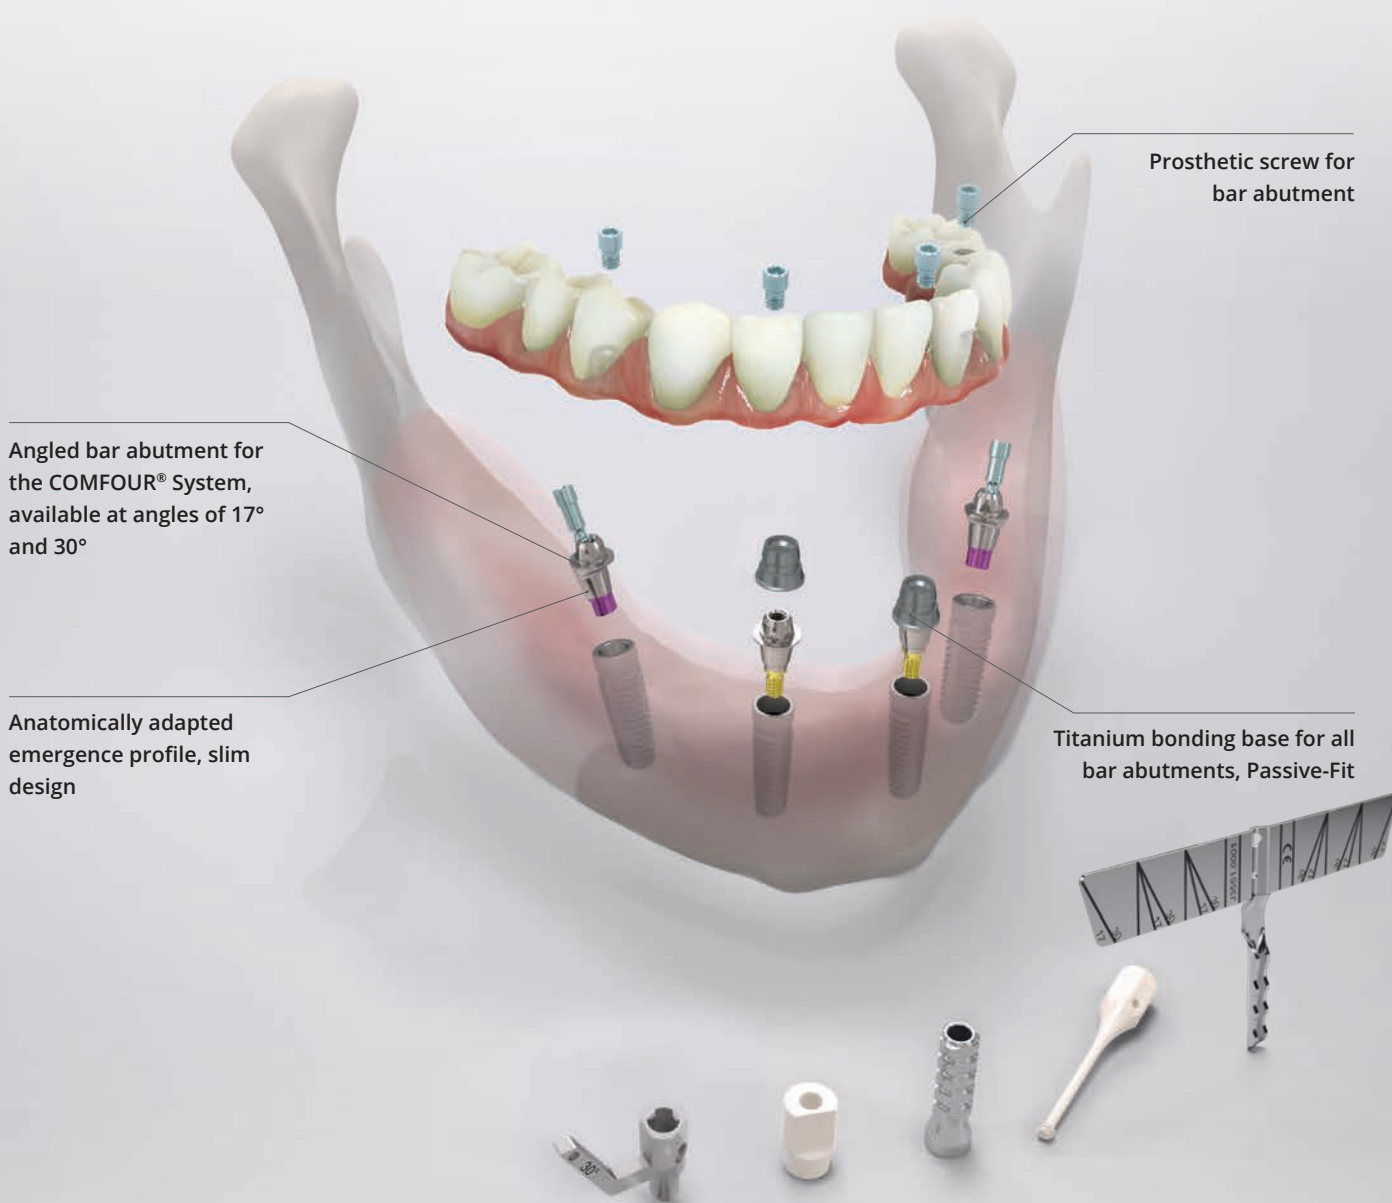

Angled bar abutment for the COMFOUR® System, available at angles of 17° and 30°

Anatomically adapted emergence profile, slim design

Titanium bonding base for all bar abutments, Passive-Fit

COMFOUR® offers a large selection of options to manage the requirements of your practice. Easier and more time-saving.

Digital service

Individually CAD/CAM fabricated prosthetics, scanning and design services, 3D implant planning, printed drilling templates and jaw models are available from Camlog through our DEDICAM® Service Division. Personal support with the accustomed competence of our employees as well as processes optimized right down to the finest detail ensure a high degree of certainty of results with the greatest possible individual freedom. Extensive libraries for the open CAD systems from 3Shape, exocad and Dental Wings are available for implant-supported restorations. Discover your options and start your digital future with DEDICAM®.


DEDICAM® Services are not available in all countries. Please ask your local Camlog representative for details.



DEDICAM®

DIGITAL CONCEPTS

Color-coding of the surgical and prosthetical CONELOG® Products



Explanation of symbols

	CE-label
	Consult instructions for use
	Caution, observe the warning notices
	Medical device
	Article number
	Lot number
	Sterilized using irradiation
	Single sterile barrier system with protective packaging outside
	Non-sterile
	Date of manufacture
	Use-by date
	Do not resterilize
	Do not reuse
	Do not use if package is damaged
	Keep away from sunlight
	Temperature limit
	Manufacturer
	MR-Conditional
	Caution: US Federal law restricts this device to sale by or on the order of a dentist or physician.

Explanation of abbreviations

∅	Diameter
A∅	Apical diameter
G∅	Gingival diameter
PP∅	Prosthetic platform diameter
L	Length
GH	Gingival height
PEEK	Poly ether ether ketone
POM	Polyoxymethylene
PPSU	Polyphenylsulfone

General safety instructions and warnings

The descriptions in this product catalog are not sufficient to allow immediate use of the CONELOG® Implant System. Instruction by a surgeon experienced in using the CONELOG® Implant System is strongly recommended.


Packaging PROGRESSIVE-LINE Implants

Secondary packaging

Sealed, folding box with color-coded product label

Inner Implant packaging (primary packaging)

Sealed, color-coded

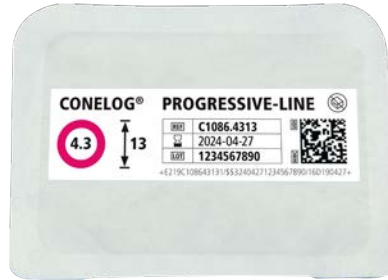

Example of product label for outer Implant packaging



Packaging SCREW-LINE Implants

Secondary packaging

Sealed, folding box with color-coded product label

Inner Implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer Implant packaging














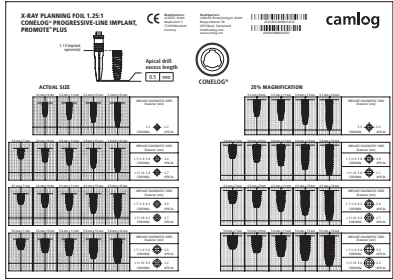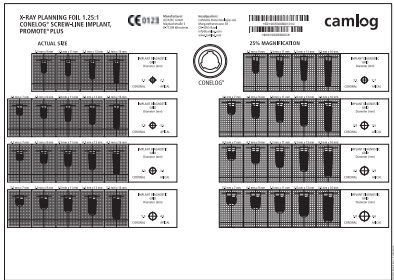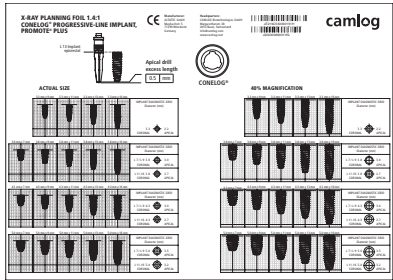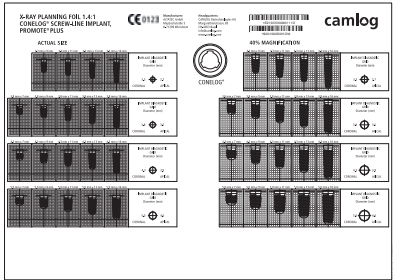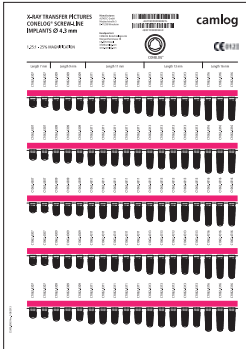

Planning

X-Ray Planning foils and X-Ray Transfer pictures

	Article	Art. No.	Ø
	X-Ray Planning foil 1.25:1 CONELOG® PROGRESSIVE-LINE Implants Magnification 25%	C5300.9014	-
	X-Ray Planning foil 1.25:1 CONELOG® SCREW-LINE Implants Magnification 25%	C5300.9010	-
	X-Ray Planning foil 1.4:1 CONELOG® PROGRESSIVE-LINE Implants Magnification 40%	C5300.9015	-
	X-Ray Planning foil 1.4:1 CONELOG® SCREW-LINE Implants Magnification 40%	C5300.9011	-
	X-Ray Transfer pictures 1.25:1 CONELOG® SCREW-LINE Implants Planning slide, self-adhesive Magnification 25%	C5300.9080	3.3 mm
		C5300.9081	3.8 mm
		C5300.9082	4.3 mm
		C5300.9083	5.0 mm

CT-Planning

for 3-D X-Ray Planning and drilling template


	Article	Art. No.	L
	<p>CT-tube for drill Ø 2.0 mm*, corrugated tubing pack of 10 internal diameter 2.1 mm external diameter 2.5 mm</p> <p>Material Titanium alloy</p>	A2002.2000	4.0 mm 10.0 mm
	<p>CT-tube for drill Ø 2.2 mm, corrugated tubing pack of 10 internal diameter 2.3 mm external diameter 2.7 mm</p> <p>Material Titanium alloy</p>	A2222.2200	4.0 mm 10.0 mm
	<p>Drill for CT-tube (for A2002.2000) Ø 2.6 mm</p> <p>Material Stainless steel</p>	A2050.2600	-
	<p>Drill for CT-tube (for A2222.2200) Ø 2.8 mm</p> <p>Material Stainless steel</p>	A2050.2800	-

* for pilot drills J5051.2003 and pilot drills SCREW-LINE J5051.2000




PROGRESSIVE-LINE

Implants with snap-in insertion post

	Article	Art. No.	Ø	L	A Ø
	CONELOG® PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1086.3309	3.3 mm	9 mm	2.2 mm
		C1086.3311		11 mm	
		C1086.3313		13 mm	
		C1086.3316		16 mm	
		C1086.3807	3.8 mm	7 mm	3.0 mm
		C1086.3809		9 mm	
		C1086.3811		11 mm	
		C1086.3813		13 mm	
		C1086.3816	4.3 mm	16 mm	2.7 mm
		C1086.4307		7 mm	
		C1086.4309		9 mm	
		C1086.4311		11 mm	
		C1086.4313	5.0 mm	13 mm	3.0 mm
		C1086.4316		16 mm	
		C1086.5007		7 mm	
		C1086.5009		9 mm	
		C1086.5011	5.0 mm	11 mm	3.5 mm
		C1086.5013		13 mm	
		C1086.5016		16 mm	
		C1086.5016		16 mm	


Surgery

Implants with screw-mounted insertion post

	Article	Art. No.	Ø	L	A Ø
	CONELOG® PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1085.3309	3.3 mm	9 mm	2.2 mm
		C1085.3311		11 mm	
		C1085.3313		13 mm	
		C1085.3316		16 mm	
		C1085.3807	3.8 mm	7 mm	3.0 mm
		C1085.3809		9 mm	
		C1085.3811		11 mm	
		C1085.3813		13 mm	
		C1085.3816	4.3 mm	16 mm	2.7 mm
		C1085.4307		7 mm	
		C1085.4309		9 mm	
		C1085.4311		11 mm	
		C1085.4313	5.0 mm	13 mm	3.0 mm
		C1085.4316		16 mm	
		C1085.5007		7 mm	
		C1085.5009		9 mm	
		C1085.5011	5.0 mm	11 mm	3.5 mm
		C1085.5013		13 mm	
		C1085.5016		16 mm	
		C1085.5016		16 mm	

PROGRESSIVE-LINE

Surgery set CAMLOG®/CONELOG®

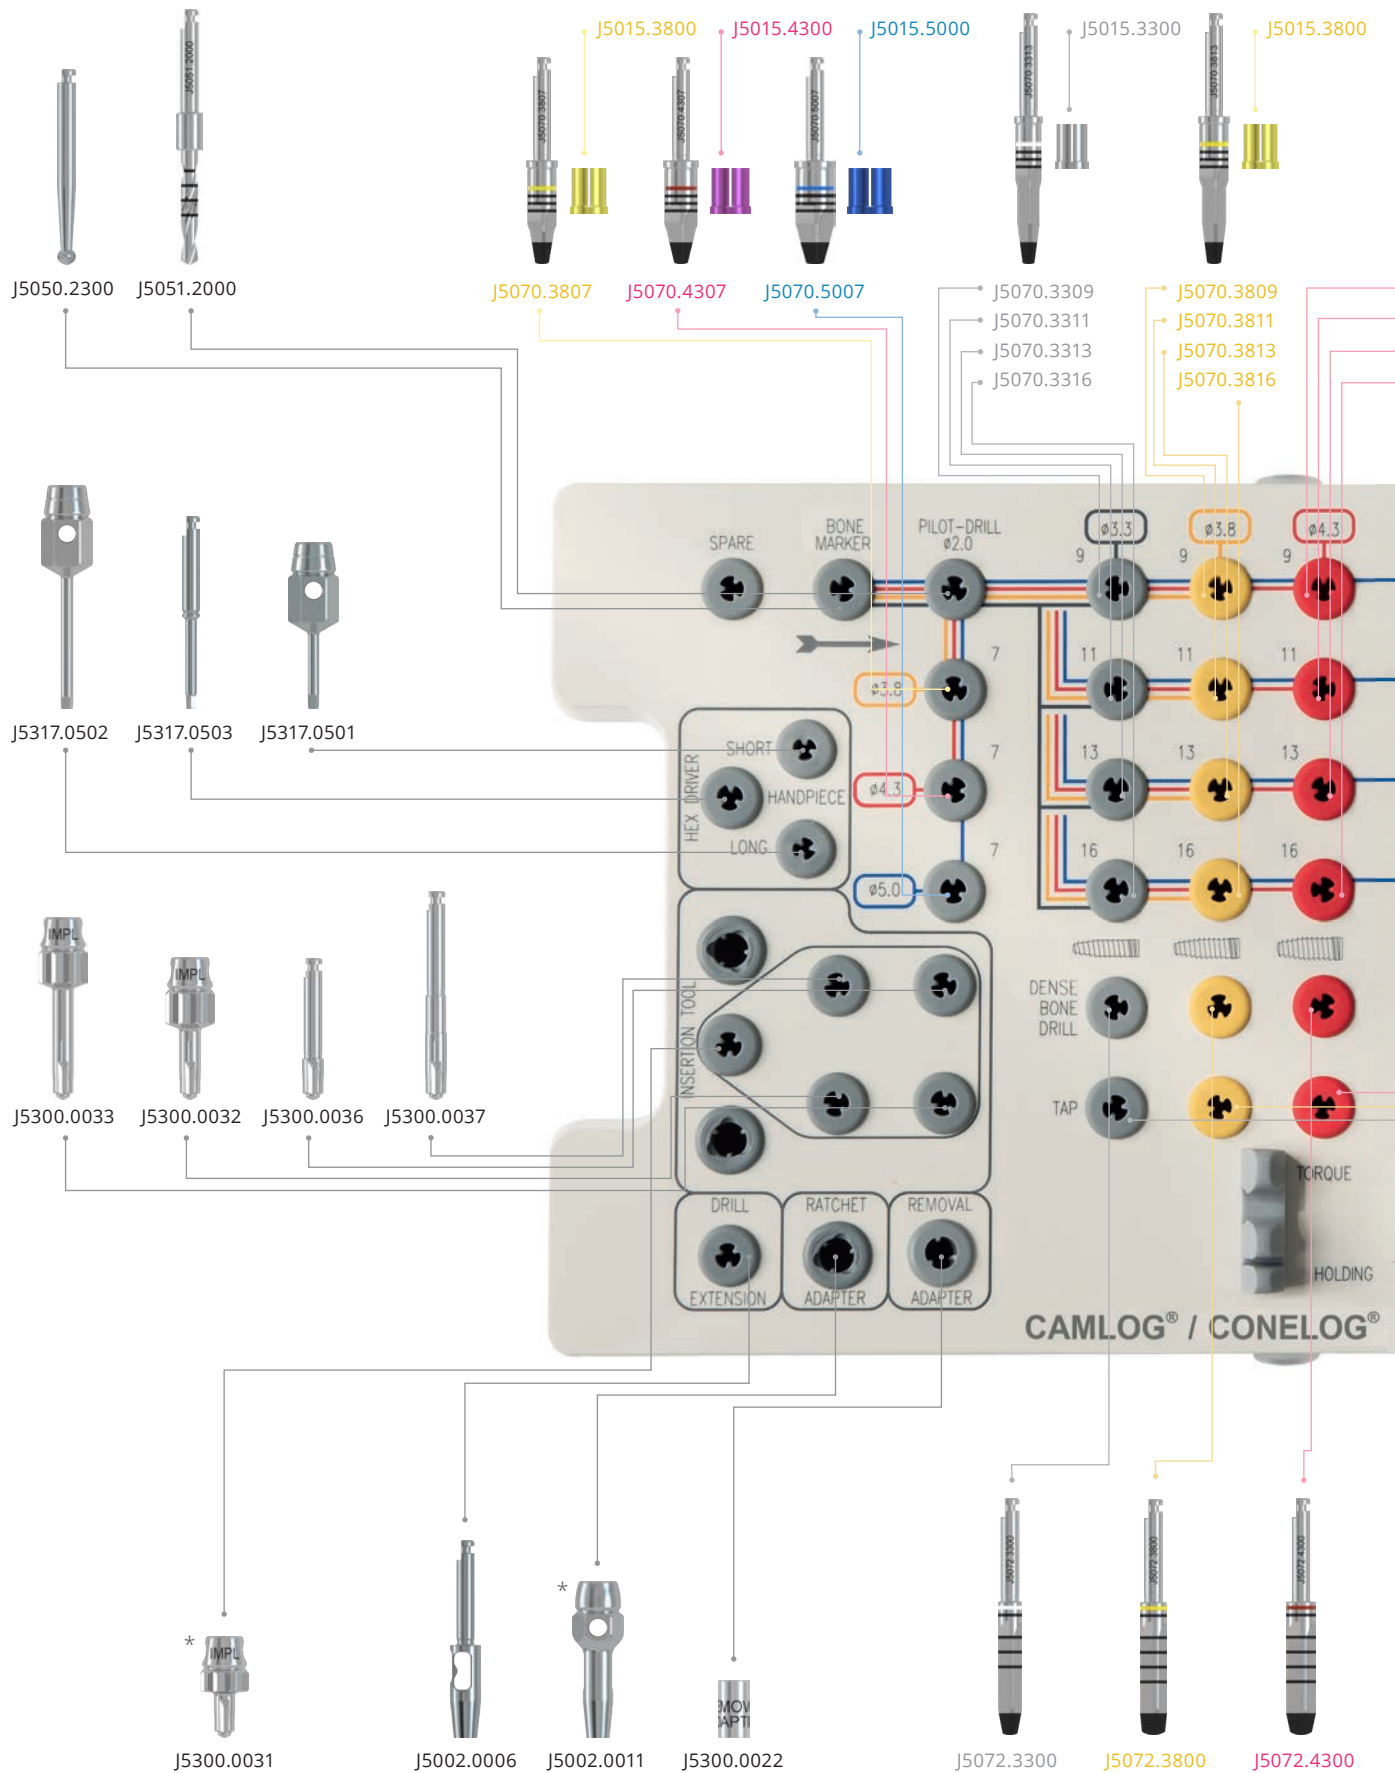


* These articles are not included in the surgery set and must be ordered separately.




The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.

Surgery

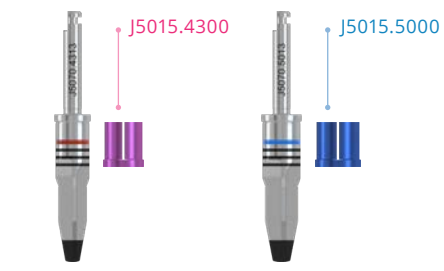

- J5070.4309
- J5070.4311
- J5070.4313
- J5070.4316
- J5070.5009
- J5070.5011
- J5070.5013
- J5070.5016

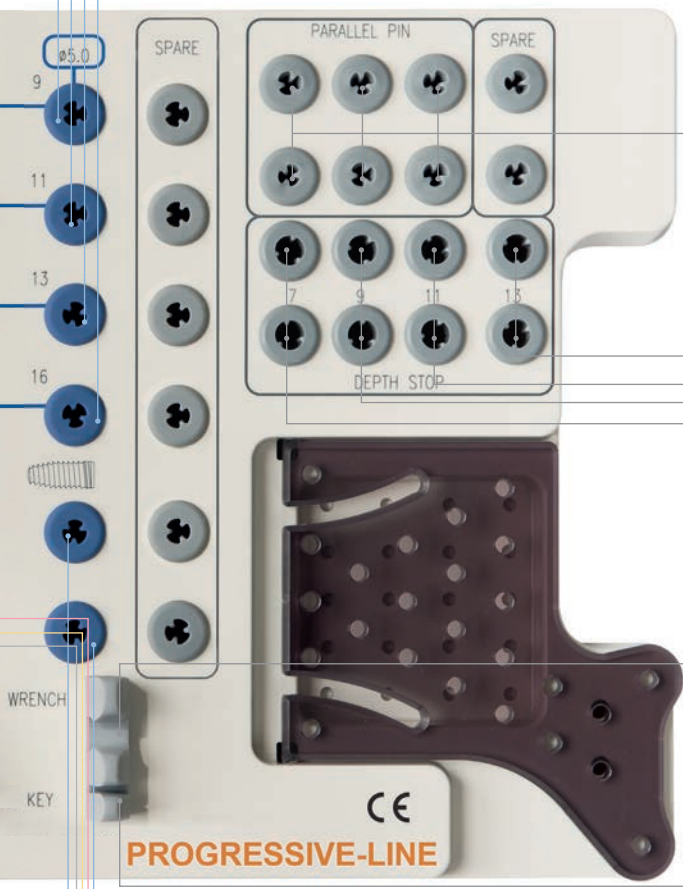

J5300.2000



J5015.0013



J5015.0011



J5015.0009



J5015.0007



J5320.1030







J5302.0010







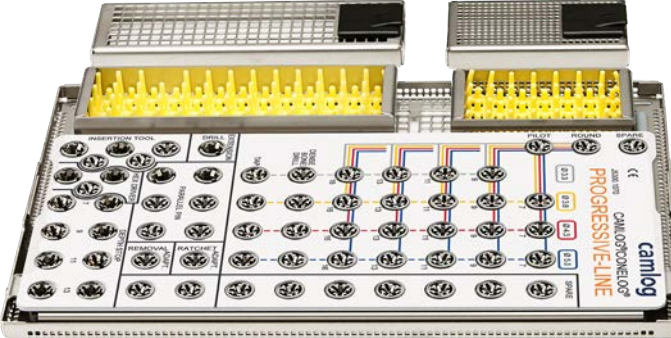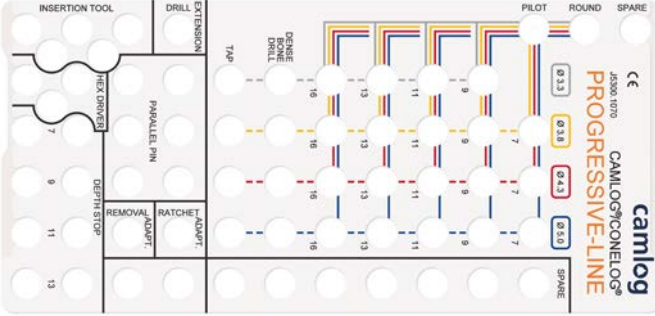

PROGRESSIVE-LINE

Surgery set

	Article	Art. No.
 <p>The image shows a complete surgery set in a white carrying case. It contains various surgical instruments including a torque wrench, a holding key, and numerous color-coded (yellow, red, blue) screws and sockets. The case is labeled 'CAMLOG® / CONELOG® PROGRESSIVE-LINE' and 'CE'.</p>	<p>Surgery set CAMLOG®/CONELOG® PROGRESSIVE-LINE contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post (taps are not included)</p>	<p>J5300.0065</p>
 <p>The image shows a surgery tray, which is a white carrying case containing the same set of color-coded surgical instruments as the full set, but without the torque wrench and holding key. It is labeled 'CAMLOG® / CONELOG® PROGRESSIVE-LINE' and 'CE'.</p>	<p>Surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE without content</p>	<p>J5300.8917</p>
 <p>The image shows a surgery wash tray, which is a white plastic tray with a grid of circular compartments. Each compartment contains a specific surgical instrument, including various sizes of screws and sockets, sorted by color and size. The tray is labeled 'CAMLOG®/CONELOG® PROGRESSIVE-LINE' and 'camlog'.</p>	<p>Surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE incl. pattern, without content</p>	<p>J5300.8970</p>
 <p>The image shows a pattern for the surgery wash tray. It is a white plastic tray with a grid of circular compartments. Each compartment is labeled with a specific instrument name and size, such as 'INSERTION TOOL', 'DRILL', 'EXTENSION', 'PARALLEL PIN', 'DEPTH STOP', 'REMOVAL ADAPT.', 'RATCHET ADAPT.', 'TAP', 'DENSE BONE', 'FINE BONE', 'PILOT', 'ROUND', and 'SPARE'. The pattern is labeled 'CAMLOG®/CONELOG® PROGRESSIVE-LINE' and 'camlog'.</p>	<p>Pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE Material PPSU</p>	<p>J5300.1070</p>


Preparation of the implant bed for CAMLOG® PROGRESSIVE-LINE Implants and for CONELOG® PROGRESSIVE-LINE Implants is performed with identical instruments.

Surgical instruments

	Article	Art. No.	Ø	L
	Form drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5070.3309	3.3 mm	9 mm
		J5070.3311		11 mm
		J5070.3313		13 mm
		J5070.3316		16 mm
		J5070.3807	3.8 mm	7 mm
		J5070.3809		9 mm
		J5070.3811		11 mm
		J5070.3813		13 mm
		J5070.3816	16 mm	
		J5070.4307	4.3 mm	7 mm
		J5070.4309		9 mm
		J5070.4311		11 mm
		J5070.4313		13 mm
		J5070.4316	16 mm	
		J5070.5007	5.0 mm	7 mm
		J5070.5009		9 mm
		J5070.5011		11 mm
J5070.5013	13 mm			
J5070.5016	16 mm			
	Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	Dense bone drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5072.3300	3.3 mm	-
		J5072.3800	3.8 mm	
		J5072.4300	4.3 mm	
		J5072.5000	5.0 mm	
	Tap PROGRESSIVE-LINE resterilizable Material Stainless steel	J5071.3300	3.3 mm	-
		J5071.3800	3.8 mm	
		J5071.4300	4.3 mm	
		J5071.5000	5.0 mm	
	Removal adapter for CAMLOG® and CONELOG® suitable for all implant diameters Material Stainless steel	J5300.0022*	3.3 mm 3.8 mm 4.3 mm 5.0 mm	6.2 mm
	Paralleling pin PROGRESSIVE-LINE with depth marks (for pilot drilling Ø 2.0 mm) Material Titanium alloy	J5300.2000	-	-

* only for use with PROGRESSIVE-LINE Implants with snap-in insertion post



PROGRESSIVE-LINE Flex
Surgery set CAMLOG®/CONELOG®

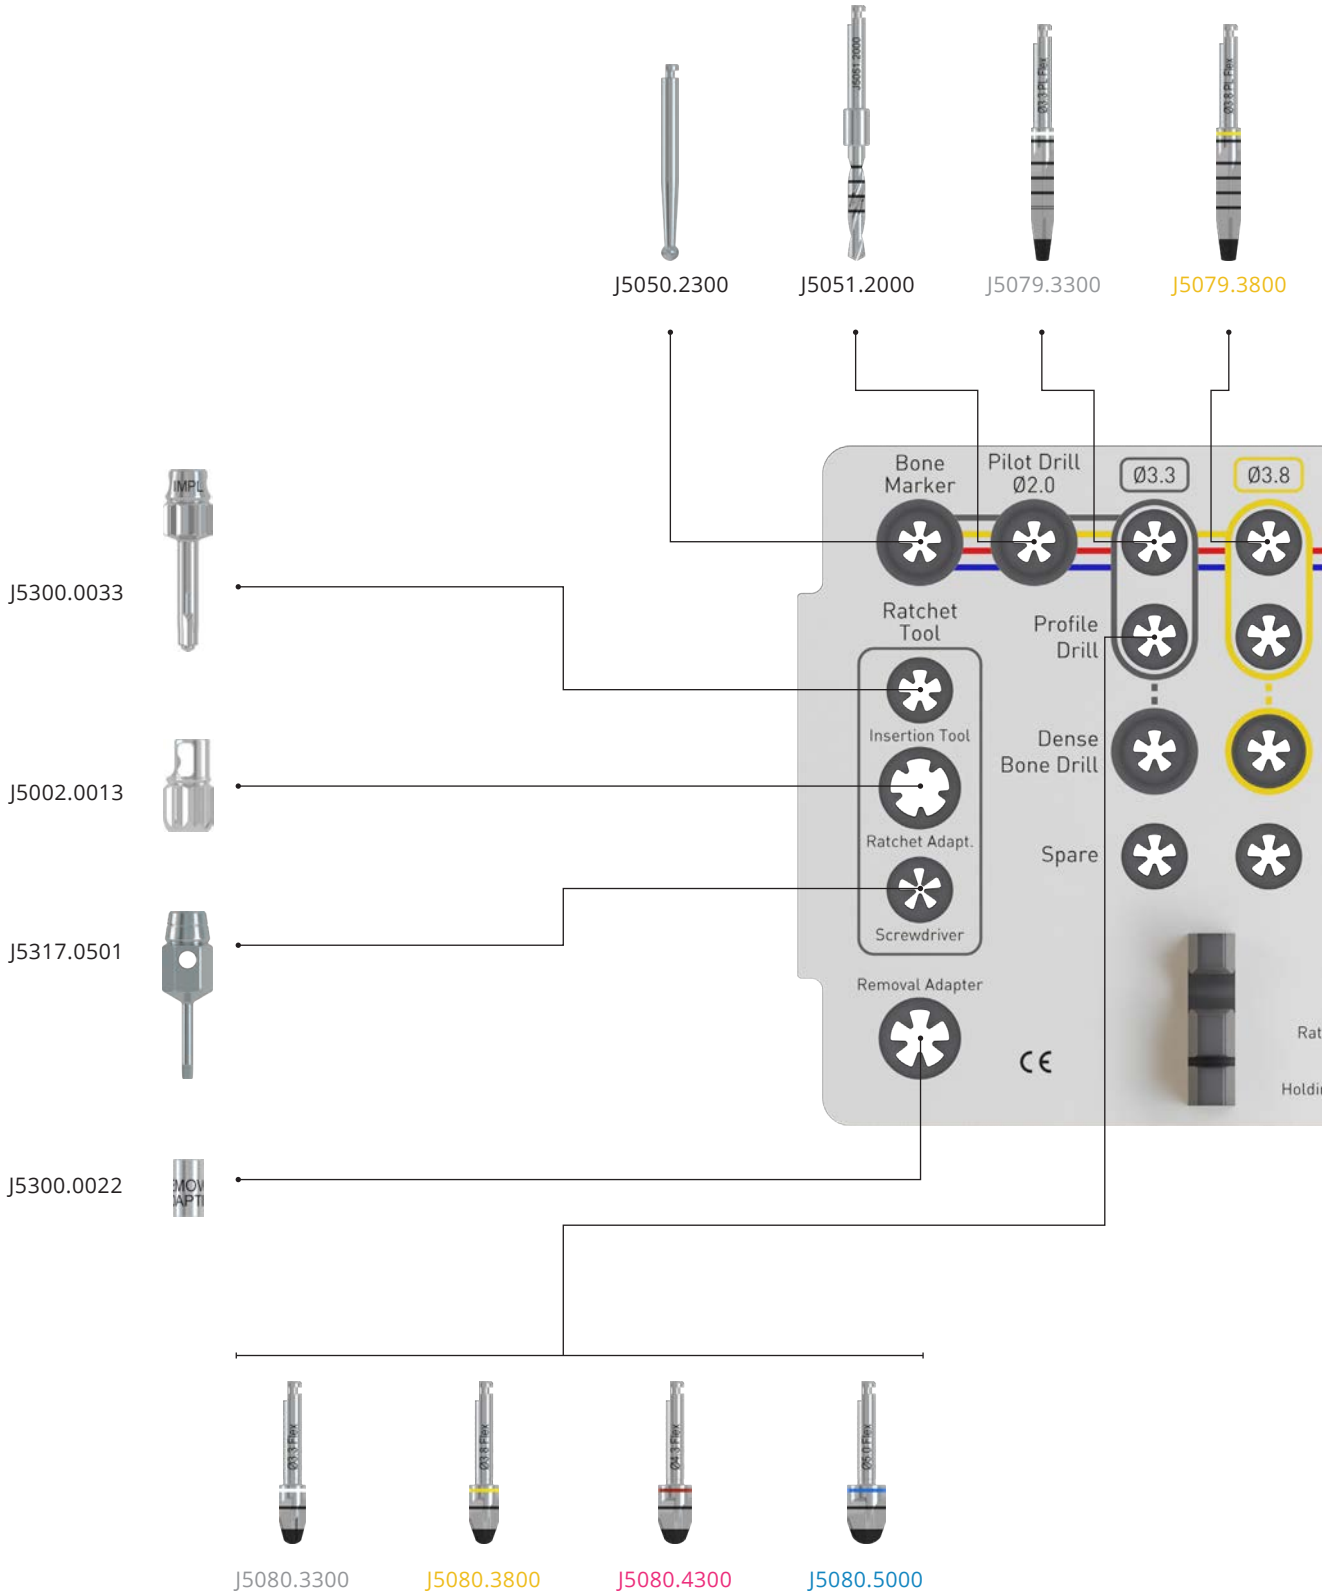

* Optional articles, can be purchased separately



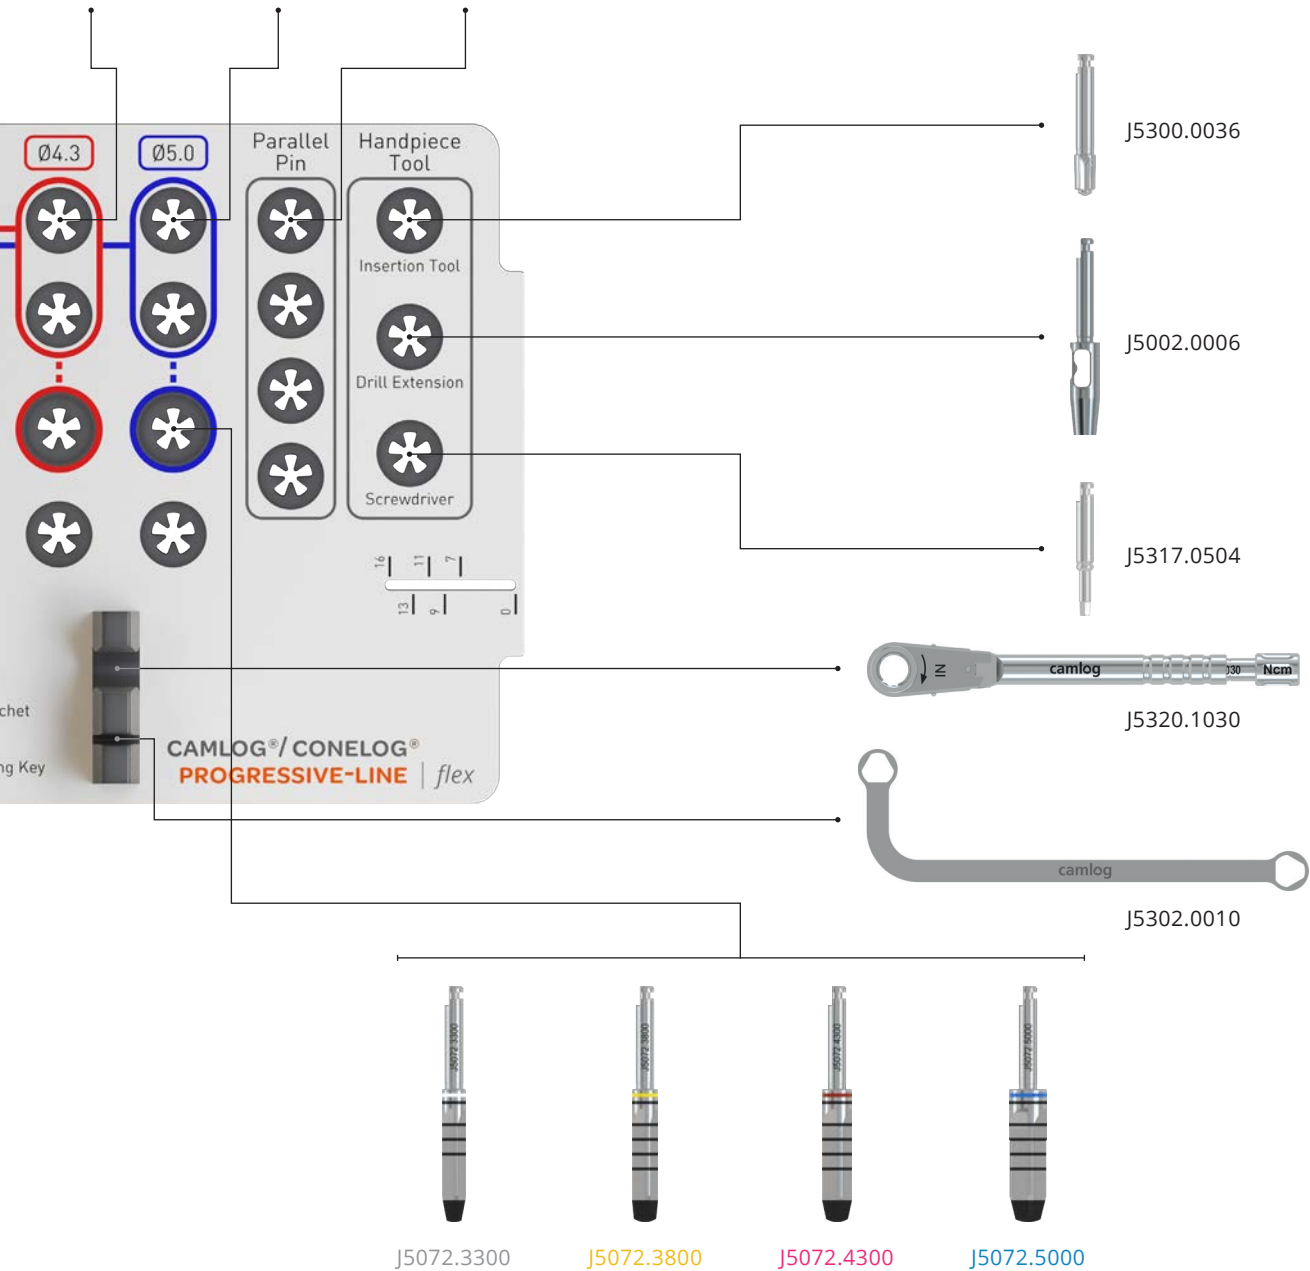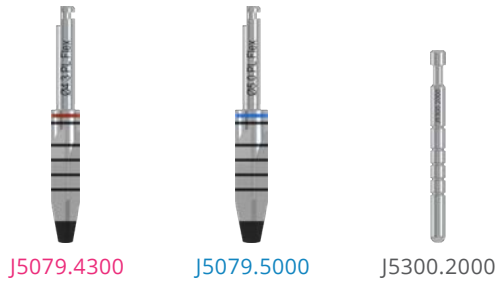

The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.






PROGRESSIVE-LINE Flex

Surgery set

	Article	Art. No.
	<p>Surgery set CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post</p>	<p>J5300.0071</p>
	<p>Surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex without content</p>	<p>J5300.8920</p>


Surgical instruments

	Article	Art. No.	Ø	L
	Drill PROGRESSIVE-LINE Flex resterilizable Material Stainless steel	J5079.3300	3.3 mm	-
		J5079.3800	3.8 mm	
		J5079.4300	4.3 mm	
		J5079.5000	5.0 mm	
	Profile drill PROGRESSIVE-LINE Flex resterilizable Material Stainless steel	J5080.3300	3.3 mm	-
		J5080.3800	3.8 mm	
		J5080.4300	4.3 mm	
		J5080.5000	5.0 mm	
	Wrench adapter Material Stainless steel	J5002.0013	-	11 mm

Preparation of the implant bed for CAMLOG® PROGRESSIVE-LINE Implants and for CONELOG® PROGRESSIVE-LINE Implants is performed with identical instruments.

PROGRESSIVE-LINE

Guide System Surgery set CAMLOG®/CONELOG®

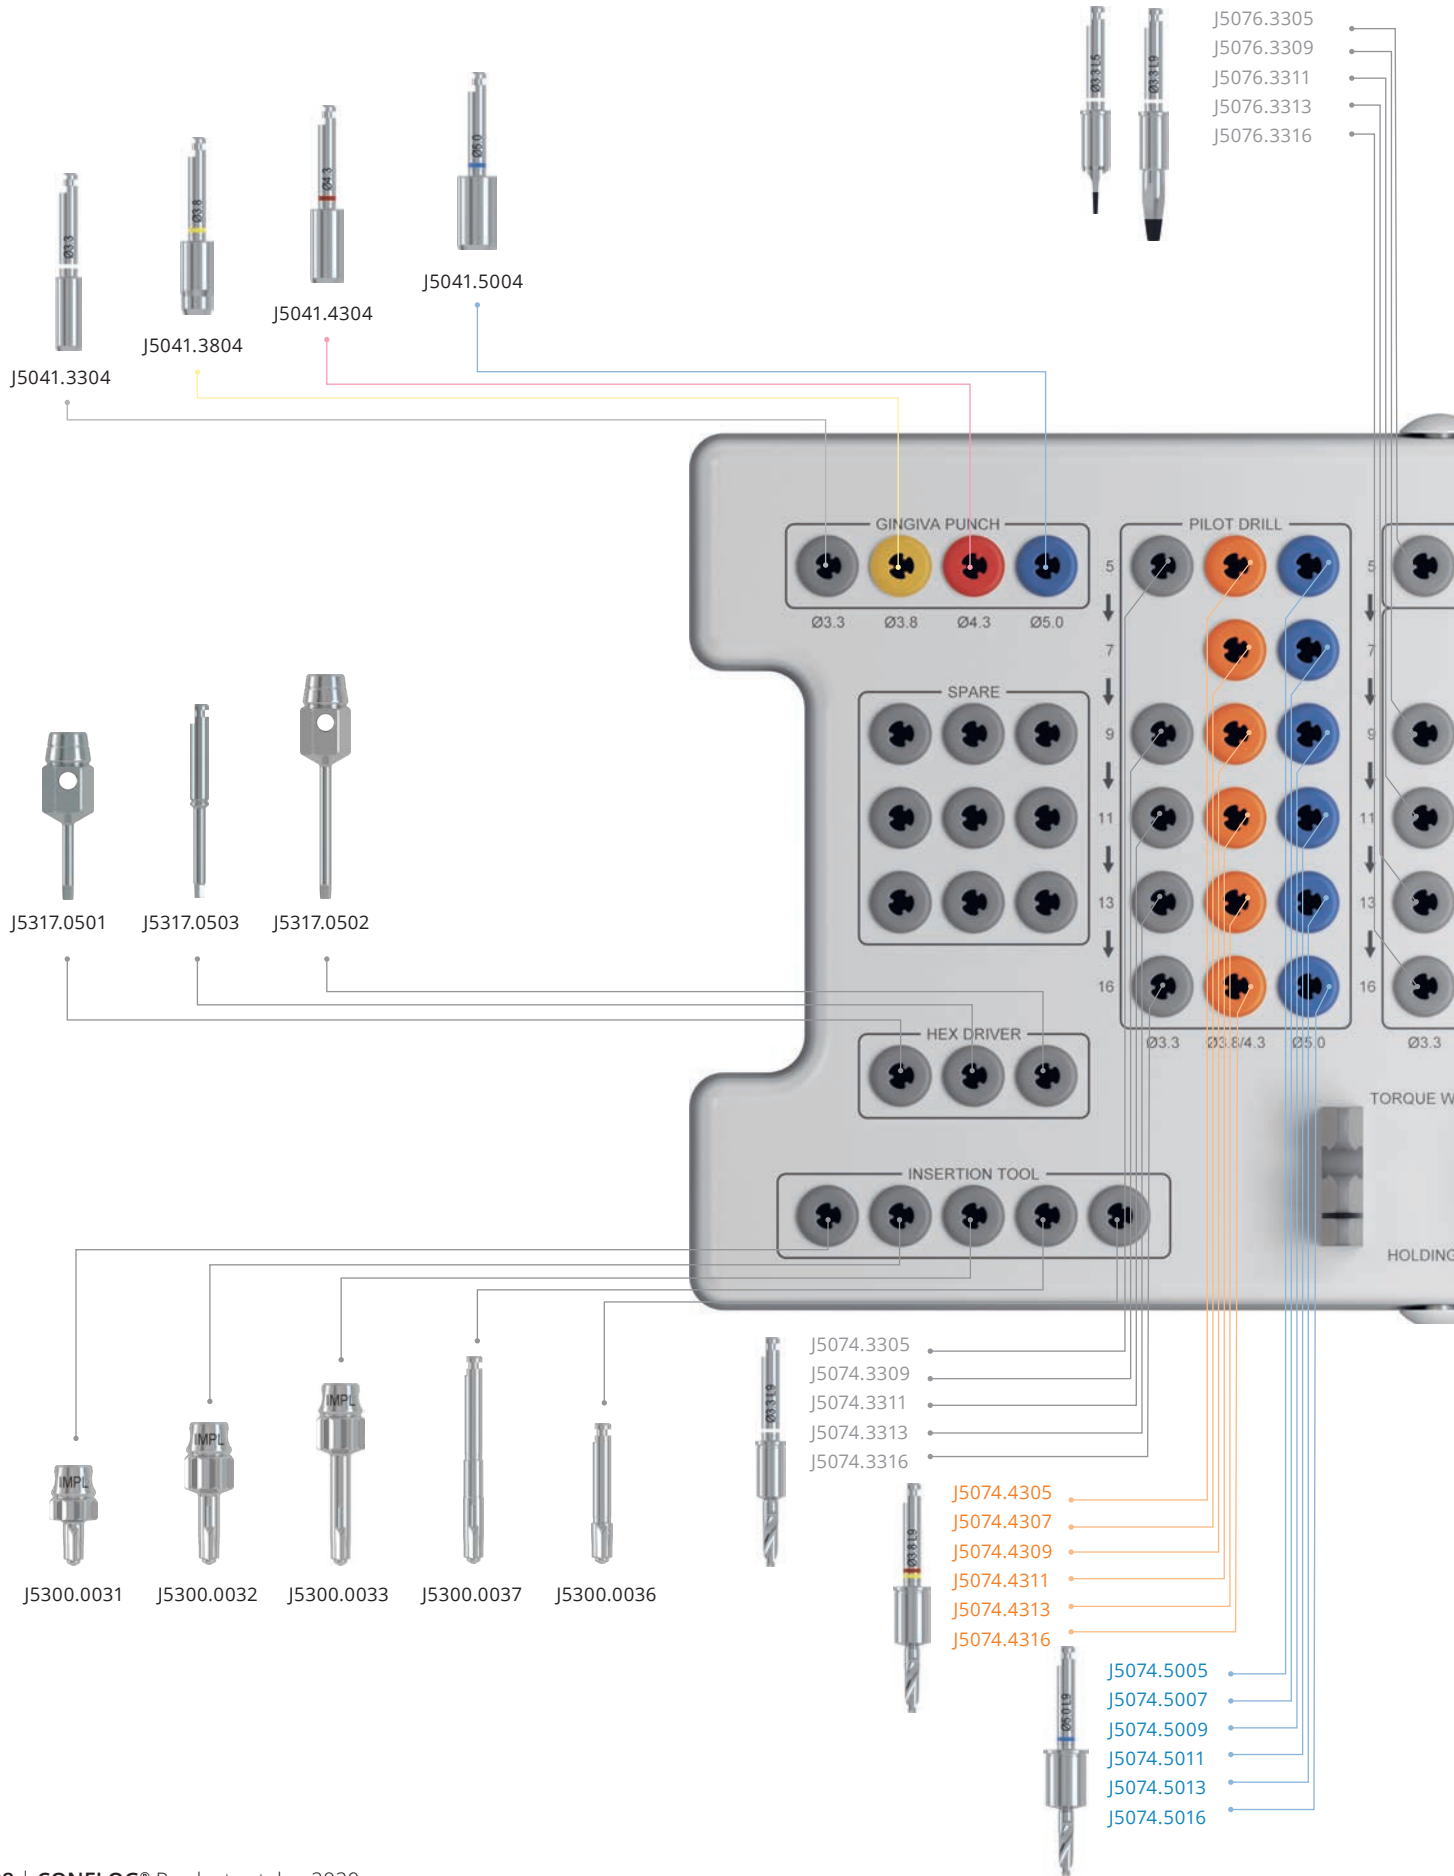



The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.

Surgery




- J5076.3805
- J5076.3807
- J5076.3809
- J5076.3811
- J5076.3813
- J5076.3816



- J5076.4305
- J5076.4307
- J5076.4309
- J5076.4311
- J5076.4313
- J5076.4316



- J5076.5005
- J5076.5007
- J5076.5009
- J5076.5011
- J5076.5013
- J5076.5016

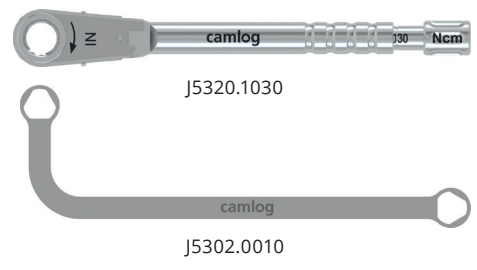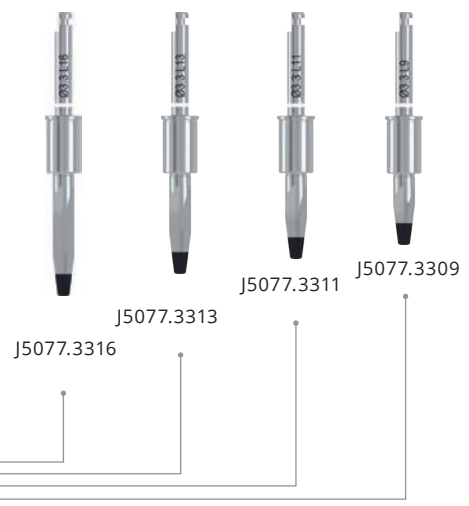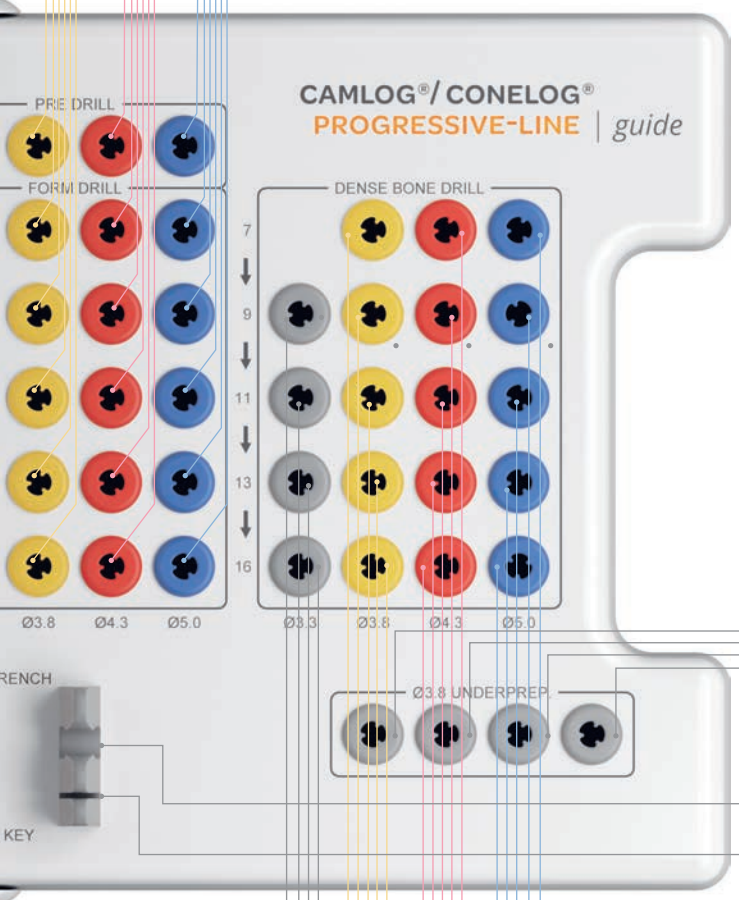

- J5078.3309
- J5078.3311
- J5078.3313
- J5078.3316

- J5078.3807
- J5078.3809
- J5078.3811
- J5078.3813
- J5078.3816

- J5078.4307
- J5078.4309
- J5078.4311
- J5078.4313
- J5078.4316



- J5078.5007
- J5078.5009
- J5078.5011
- J5078.5013
- J5078.5016



PROGRESSIVE-LINE

Guide System





	Article	Art. No.
	<p>Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE without content</p>	<p>J5300.8919</p>

	Article	Art. No.	Ø	L
	<p>Guide System gingiva punch PROGRESSIVE-LINE resterilizable</p> <p>Material Stainless steel</p>	J5041.3304	3.3 mm	-
		J5041.3804	3.8 mm	
		J5041.4304	4.3 mm	
		J5041.5004*	5.0 mm	
	<p>Guide System pilot drill PROGRESSIVE-LINE resterilizable</p> <p>Material Stainless steel</p>	J5074.3305	3.3 mm	5 mm
		J5074.3309		9 mm
		J5074.3311		11 mm
		J5074.3313		13 mm
		J5074.3316		16 mm
		J5074.4305	3.8 mm	5 mm
		J5074.4307		7 mm
		J5074.4309	3.8 mm	9 mm
		J5074.4311		11 mm
		J5074.4313		13 mm
		J5074.4316		16 mm
		J5074.5005*	5.0 mm	5 mm
		J5074.5007*		7 mm
		J5074.5009*		9 mm
		J5074.5011*		11 mm
		J5074.5013*		13 mm
J5074.5016*	16 mm			

* product availability expected for end of Q1/2021

Notes






CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1085.xxxx with screw-mounted insertion post can be used with the PROGRESSIVE-LINE Guide System.

	Article	Art. No.	Ø	L
	Guide System pre-drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5076.3305	3.3 mm	5 mm
		J5076.3805	3.8 mm	
		J5076.4305	4.3 mm	
		J5076.5005*	5.0 mm	
	Guide System form drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5076.3309	3.3 mm	9 mm
		J5076.3311		11 mm
		J5076.3313		13 mm
		J5076.3316		16 mm
		J5076.3807	3.8 mm	7 mm
		J5076.3809		9 mm
		J5076.3811		11 mm
		J5076.3813	4.3 mm	13 mm
		J5076.3816		16 mm
		J5076.4307		7 mm
		J5076.4309	4.3 mm	9 mm
		J5076.4311		11 mm
		J5076.4313		13 mm
		J5076.4316		16 mm
		J5076.5007*	5.0 mm	7 mm
		J5076.5009*		9 mm
J5076.5011*	11 mm			
J5076.5013*	13 mm			
J5076.5016*		16 mm		
	Guide System dense bone drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5078.3309	3.3 mm	9 mm
		J5078.3311		11 mm
		J5078.3313		13 mm
		J5078.3316		16 mm
		J5078.3807	3.8 mm	7 mm
		J5078.3809		9 mm
		J5078.3811		11 mm
		J5078.3813	4.3 mm	13 mm
		J5078.3816		16 mm
		J5078.4307		7 mm
		J5078.4309	4.3 mm	9 mm
		J5078.4311		11 mm
		J5078.4313		13 mm
		J5078.4316		16 mm
		J5078.5007*	5.0 mm	7 mm
		J5078.5009*		9 mm
J5078.5011*	11 mm			
J5078.5013*	13 mm			
J5078.5016*		16 mm		
	Guide System form drill for Ø 3.8 mm under preparation PROGRESSIVE-LINE resterilizable Material Stainless steel	J5077.3309	3.3 mm	9 mm
		J5077.3311		11 mm
		J5077.3313		13 mm
		J5077.3316		16 mm

* product availability expected for end of Q1/2021

PROGRESSIVE-LINE

Guide System


	Article	Art. No.	Ø	L
	Guide System template drill PROGRESSIVE-LINE for Guide System guiding sleeve Material Stainless steel	J3753.3300	3.3 mm	-
		J3753.4300	3.8 mm 4.3 mm	
		J3753.5000*	5.0 mm	
	Guide System guiding sleeve PROGRESSIVE-LINE** (2 units) Material Titanium alloy	J3754.3301	3.3 mm	-
		J3754.3801	3.8 mm	
		J3754.4301	4.3 mm	
		J3754.5001*	5.0 mm	
	Guide System setting tool PROGRESSIVE-LINE for Guide System guiding sleeve Material Stainless steel	J3717.3300	3.3 mm	-
		J3717.4300	3.8 mm 4.3 mm	
		J3717.5000*	5.0 mm	
	Guide System check-up pin PROGRESSIVE-LINE for Guide System guiding sleeve Material Stainless steel	J5301.3310	3.3 mm	-
		J5301.4310	3.8 mm 4.3 mm	
		J5301.5010*	5.0 mm	
	Guide System CONELOG® Insertion post, screw-mounted for CONELOG® Lab implant/implant analog, incl. fixing screw (2 units) Material Titanium alloy	C2026.3303	3.3 mm	-
		C2026.3803	3.8 mm	
		C2026.4303	4.3 mm	
		C2026.5003*	5.0 mm	

* product availability expected for end of Q1/2021

** only for use with PROGRESSIVE-LINE Implants with screw-mounted insertion post


SCREW-LINE

Implants with snap-in insertion post

	Article	Art. No.	Ø	L	A Ø
	CONELOG® SCREW-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1066.3309*	3.3 mm	9 mm	2.7 mm
		C1066.3311*		11 mm	
		C1066.3313*		13 mm	
		C1066.3316*		16 mm	
		C1066.3807*	3.8 mm	7 mm	3.5 mm
		C1066.3809*		9 mm	
		C1066.3811*		11 mm	
		C1066.3813*		13 mm	
		C1066.3816*	16 mm	3.9 mm	
		C1066.4307*	7 mm		
		C1066.4309*	9 mm		
		C1066.4311*	11 mm		
		C1066.4313*	13 mm	4.6 mm	
		C1066.4316*	16 mm		
		C1066.5007*	7 mm		
		C1066.5009*	9 mm		
		C1066.5011*	5.0 mm	11 mm	4.6 mm
		C1066.5013*		13 mm	
C1066.5016*	16 mm				

* Please note: CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1066.xxxx succeed Implants with Art. No. C1064.xxxx starting in October 2020. Depending on your country CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1064.xxxx might still be available for a longer period.

Implants with screw-mounted insertion post


	Article	Art. No.	Ø	L	A Ø
	CONELOG® SCREW-LINE Implant, Promote® plus incl. screw-mounted insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1065.3309**	3.3 mm	9 mm	2.7 mm
		C1065.3311**		11 mm	
		C1065.3313**		13 mm	
		C1065.3316**		16 mm	
		C1065.3807**	3.8 mm	7 mm	3.5 mm
		C1065.3809**		9 mm	
		C1065.3811**		11 mm	
		C1065.3813**		13 mm	
		C1065.3816**	16 mm	3.9 mm	
		C1065.4307**	7 mm		
		C1065.4309**	9 mm		
		C1065.4311**	11 mm		
		C1065.4313**	13 mm	4.6 mm	
		C1065.4316**	16 mm		
		C1065.5007**	7 mm		
		C1065.5009**	9 mm		
		C1065.5011**	5.0 mm	11 mm	4.6 mm
		C1065.5013**		13 mm	
C1065.5016**	16 mm				

** Please note: CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1065.xxxx succeed Implants with Art. No. C1063.xxxx starting in October 2020. Depending on your country CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1063.xxxx might still be available for a longer period.

Notes


CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1064.xxxx and Art. No. C1065.xxxx can be used exclusively with the drivers Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034, J5300.0035, J5300.0036 or J5300.0037.

Surgery

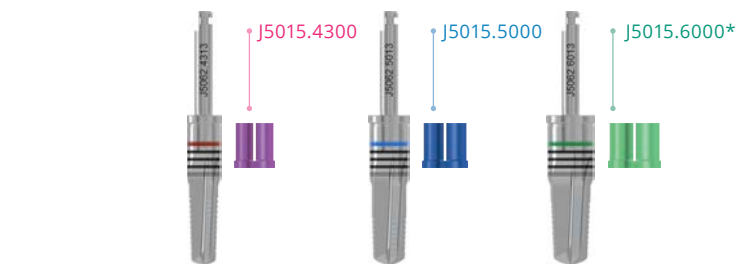

The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.

- J5062.4309
- J5062.4311
- J5062.4313
- J5062.4316
- J5062.5009
- J5062.5011
- J5062.5013
- J5062.5016
- J5062.6009*
- J5062.6011*
- J5062.6013*
- J5062.6016*

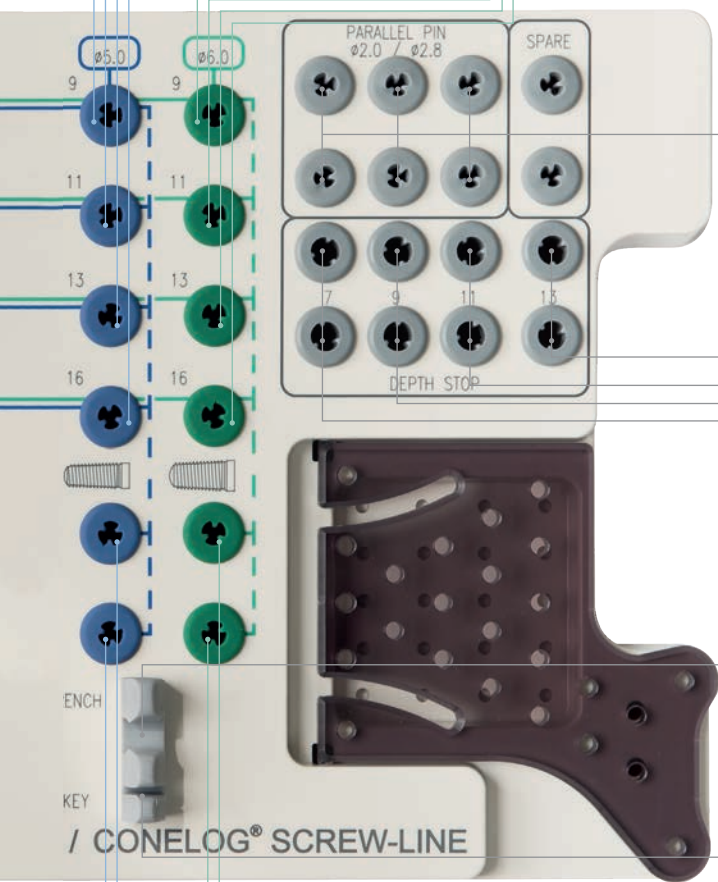

J5300.2028




J5015.0013 J5015.0011 J5015.0009 J5015.0007



J5320.1030



J5302.0010

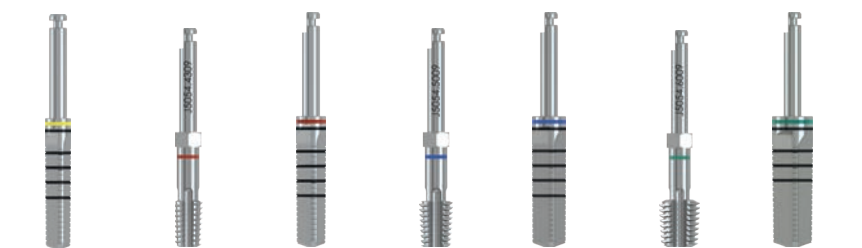

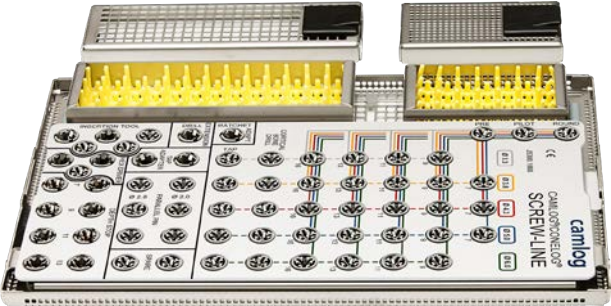
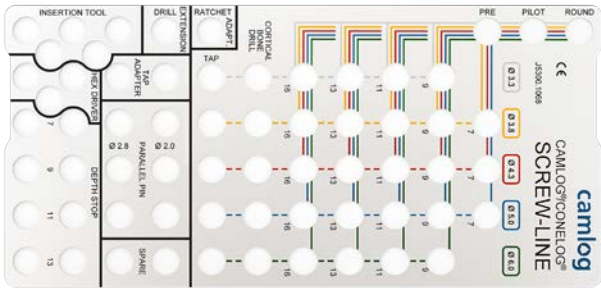


J5053.3816 J5054.4309 J5053.4316 J5054.5009 J5053.5016 J5054.6009* J5053.6016*

* only for CAMLOG® SCREW-LINE Implants Ø 6.0 mm



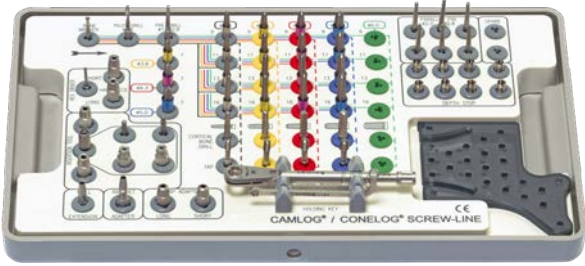

SCREW-LINE

Surgery set

	Article	Art. No.
	<p>Surgery set CAMLOG®/CONELOG® SCREW-LINE contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post (drills and taps for Ø 6.0 mm are not included)</p>	<p>J5300.0063</p>
	<p>Surgery tray CAMLOG®/CONELOG® SCREW-LINE without content</p>	<p>J5300.8916</p>
	<p>Surgery wash tray CAMLOG®/CONELOG® SCREW-LINE incl. pattern, without content</p>	<p>J5300.8968</p>
	<p>Pattern for surgery wash tray CAMLOG®/CONELOG® SCREW-LINE</p> <p>Material Aluminum</p>	<p>J5300.1068</p>


Preparation of the implant bed for CAMLOG® SCREW-LINE Implants and for CONELOG® SCREW-LINE Implants is performed with identical instruments.

Surgical instruments

	Article	Art. No.	Ø	L
	Form drill SCREW-LINE resterilizable Material Stainless steel	J5062.3309	3.3 mm	9 mm
		J5062.3311		11 mm
		J5062.3313		13 mm
		J5062.3316		16 mm
		J5062.3807	3.8 mm	7 mm
		J5062.3809		9 mm
		J5062.3811		11 mm
		J5062.3813		13 mm
		J5062.3816		16 mm
		J5062.4307	4.3 mm	7 mm
		J5062.4309		9 mm
		J5062.4311		11 mm
		J5062.4313		13 mm
		J5062.4316	16 mm	
		J5062.5007	5.0 mm	7 mm
		J5062.5009		9 mm
		J5062.5011		11 mm
		J5062.5013		13 mm
J5062.5016	16 mm			
	Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	Form drill SCREW-LINE Cortical bone resterilizable Material Stainless steel	J5053.3316	3.3 mm	-
		J5053.3816	3.8 mm	
		J5053.4316	4.3 mm	
		J5053.5016	5.0 mm	
	Tap SCREW-LINE with hexagon, resterilizable Material Stainless steel	J5054.3309	3.3 mm	-
		J5054.3809	3.8 mm	
		J5054.4309	4.3 mm	
		J5054.5009	5.0 mm	




SCREW-LINE

Guide System

	Article	Art. No.	Ø	L
	<p>Guide System pilot drill set internal irrigation, sterile (for pilot drills Ø 2.0 mm)</p> <p>Material Stainless steel</p>	J5063.3309	3.3 mm	9 mm (incl. 5 mm)**
		J5063.3311		11 mm (incl. 5 and 9 mm)**
		J5063.3313		13 mm (incl. 5, 9 and 11 mm)**
		J5064.3316*		16 mm
		J5063.4307	3.8 mm	7 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4309	3.8 mm	9 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4311	3.8 mm	11 mm (incl. 5 and 9 mm)**
			4.3 mm	
		J5063.4313	3.8 mm	13 mm (incl. 5, 9 and 11 mm)**
			4.3 mm	
		J5064.4316*	3.8 mm	16 mm
			4.3 mm	

* Necessary Guide System pilot drill for implant length 16 mm, following obligatory prior use of the pilot drill set length 13 mm.

** All Guide System pilot drill sets include a 5 mm long pilot drill, as well as all pilot drills necessary for the selected implant length.
All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

	Article	Art. No.	Ø	L		
	Guide System surgery set, SCREW-LINE internal irrigation, sterile Material Stainless steel	J5065.3309	3.3 mm	9 mm (incl. 5 mm)**		
		J5065.3311		11 mm (incl. 5 and 9 mm)**		
		J5065.3313		13 mm (incl. 5, 9 and 11 mm)**		
		J5066.3316*		16 mm		
		J5065.3807	3.8 mm	7 mm (incl. 5 mm)**		
		J5065.3809		9 mm (incl. 5 mm)**		
		J5065.3811		11 mm (incl. 5 and 9 mm)**		
		J5065.3813		13 mm (incl. 5, 9 and 11 mm)**		
		J5066.3816*	4.3 mm	16 mm		
		J5065.4307		7 mm (incl. 5 mm)**		
		J5065.4309		9 mm (incl. 5 mm)**		
		J5065.4311		11 mm (incl. 5 and 9 mm)**		
		J5065.4313	13 mm (incl. 5, 9 and 11 mm)**			
		J5066.4316*	16 mm			
			Guide System form drill, SCREW-LINE, cortical bone internal irrigation, sterile Material Stainless steel	J5068.3309	3.3 mm	9 mm
				J5068.3311		11 mm
J5068.3313	13 mm					
J5068.3316	16 mm					
J5068.3807	3.8 mm			7 mm		
J5068.3809				9 mm		
J5068.3811				11 mm		
J5068.3813				13 mm		
J5068.3816	4.3 mm			16 mm		
J5068.4307				7 mm		
J5068.4309				9 mm		
J5068.4311				11 mm		
J5068.4313	13 mm					
J5068.4316	16 mm					
	Guide System gingiva punch sterile Material Stainless steel	J5041.3303	3.3 mm	-		
		J5041.3803	3.8 mm			
		J5041.4303	4.3 mm			





* Necessary Guide System form drill for implant length 16 mm, following obligatory prior use of the Guide System surgery set length 13 mm.

** All Guide System surgery sets include a 5 mm long pre-drill, as well as all form drills necessary for the selected implant length.





All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

SCREW-LINE

Guide System






	Article	Art. No.	Ø	L
	Guide System guiding sleeve height 3.0 mm (2 units) Material Titanium alloy	J3734.3303*	3.3 mm	-
		J3734.3803*	3.8 mm	
		J3734.4303*	4.3 mm	
	Guide System CONELOG® Insertion post, screw-mounted for CONELOG® Lab implant/implant analog, incl. fixing screw (2 units) Material Titanium alloy	C2026.3303	3.3 mm	-
		C2026.3803	3.8 mm	
		C2026.4303	4.3 mm	
	Guide System template drill for Guide System guiding sleeve Material Stainless steel	J3733.3300	3.3 mm	-
		J3733.4300	3.8 mm	
			4.3 mm	
	Guide System seating tool for Guide System guiding sleeve Material Stainless steel	J3716.3300	3.3 mm	-
		J3716.4300	3.8 mm	
			4.3 mm	

* only for use with SCREW-LINE Implants with screw-mounted insertion post
All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.






	Article	Art. No.	Ø	L
	Guide System check-up pin for Guide System guiding sleeve Material Stainless steel	J5301.3300	3.3 mm	
		J5301.4300	3.8 mm	-
			4.3 mm	
	Guide System driver* for Guide System implant Ø 3.3/3.8/4.3 mm, manual/wrench Material Stainless steel	J5303.4300	3.3 mm 3.8 mm 4.3 mm	-
	Guide System driver* for Guide System implant Ø 3.3/3.8/4.3 mm, with ISO shaft for angled hand piece Material Stainless steel	J5304.4300	3.3 mm 3.8 mm 4.3 mm	-
	Drill extension ISO shaft, for instruments with internal irrigation Material Stainless steel	J5002.0005	-	26.6 mm

* only for use with CONELOG® SCREW-LINE Implants with Art. No. C1063.xxxx.

General surgical instruments

	Article	Art. No.	Ø	L
	Round bur resterilizable Material Stainless steel	J5050.2300	2.3 mm	-
	Point drill resterilizable Material Stainless steel	B1012*	1.5 mm	30.0 mm
	Pilot drill without coil, resterilizable Material Stainless steel	J5051.2003	2.0 mm	-
	Pilot drill SCREW-LINE resterilizable Material Stainless steel	J5051.2000	2.0 mm	-
	Pre-drill SCREW-LINE resterilizable Material Stainless steel	J5051.2800	1.7 – 2.8 mm	-

* Manufacturer: AXIS bidental SA, Les Rosées 5, 2336 Les Bois, Switzerland

	Article	Art. No.	Ø	L	
	Depth stop SCREW-LINE for pilot drill (J5051.2000) and pre-drill (J5051.2800), resterilizable Material Stainless steel	J5015.0007	-	7 mm	
		J5015.0009		9 mm	
		J5015.0011		11 mm	
		J5015.0013		13 mm	
	Bone profiler Material Stainless steel	Ø 5.0 mm	J5003.3350	3.3 mm	-
		Ø 6.0 mm	J5003.4360	3.8 mm 4.3 mm	
		Ø 7.0 mm	J5003.5070	5.0 mm	
	CONELOG® Guiding pin for bone profiler Material Titanium alloy		C5002.3300	3.3 mm	-
			C5002.3800	3.8 mm	
			C5002.4300	4.3 mm	
			C5002.5000	5.0 mm	
	Countersink Material Stainless steel	Ø 4.6 mm	J5006.3346	3.3 mm	-
		Ø 5.2 mm	J5006.3852	3.8 mm	
		Ø 5.6 mm	J5006.4356	4.3 mm	
		Ø 6.3 mm	J5006.5063	5.0 mm	
	Baring drill for cover screw Material Stainless steel		J5004.3300	3.3 mm	-
			J5004.3800	3.8 mm	
			J5004.4300	4.3 mm	
			J5004.5000	5.0 mm	




General surgical instruments

	Article	Art. No.	Dimension
	<p>Paralleling pin SCREW-LINE with depth marks</p> <p>Material Titanium alloy</p>	J5300.2028	<p>∅ 1.7 – 2.8 mm/ 2.0 mm</p>
	<p>Drill extension ISO shaft (not for instruments with internal irrigation)</p> <p>Material Stainless steel</p>	J5002.0006	26.5 mm
	<p>Tap adapter, short for tap SCREW-LINE</p> <p>Material Stainless steel</p>	J5322.0010	18.0 mm
	<p>Tap adapter, long for tap SCREW-LINE</p> <p>Material Stainless steel</p>	J5322.0011	23.0 mm

	Article	Art. No.	Dimension
	Driver, extra short for screw implants, manual/wrench Material Stainless steel	J5300.0031*	13.7 mm
	Driver, short for screw implants, manual/wrench Material Stainless steel	J5300.0032*	19.2 mm
	Driver, long for screw implants, manual/wrench Material Stainless steel	J5300.0033*	24.8 mm
	Driver, short for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft) Material Stainless steel	J5300.0036*	19.1 mm
	Driver, long for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft) Material Stainless steel	J5300.0037*	28.2 mm
	Driver, short for screw implants, with ISO-shaft for angled hand piece (with hexagon at the shaft) Material Stainless steel	J5300.0034*	19.1 mm
	Driver, long for screw implants, with ISO-shaft for angled hand piece (with hexagon at the shaft) Material Stainless steel	J5300.0035*	28.2 mm








* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1086.xxxx and CONELOG® SCREW-LINE Implants with Art. No. C1064.xxxx, C1065.xxxx and C1066.xxxx.

General surgical instruments






	Article	Art. No.	Dimension
	<p>Cardanic driver (30°) for screw implants, adjustable length</p> <p>Material Stainless steel</p>	J5300.0038*	-
	<p>PickUp instrument holder for carrying implants</p> <p>Material Stainless steel</p>	J5300.0030**	-
	<p>Adapter ISO shaft for angled hand piece</p> <p>Material Stainless steel</p>	J5002.0011	21.0 mm

* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1086.xxxx and CONELOG® SCREW-LINE Implants with Art. No. C1064.xxxx, C1065xxxx and C1066.xxxx.

** only for use with CONELOG® PROGRESSIVE-LINE Implants (with snap-in insertion post) with Art. No. C1086.xxxx and CONELOG® SCREW-LINE Implants with Art. No. C1062.xxxx and C1066.xxxx.


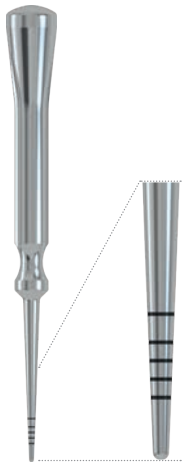
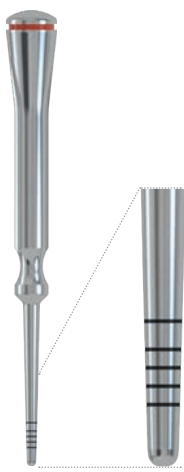
	Article	Art. No.	Ø	Dimension
	Holding key for insertion post Material Stainless steel	J5302.0010	-	-
	CONELOG® Adapter for screw implants, short for CONELOG® Implants Material Stainless steel	C5302.3311	3.3 mm	28.1 mm
		C5302.4311	3.8 mm	
			4.3 mm	
		C5302.5011	5.0 mm	
	CONELOG® Adapter for screw implants, long for CONELOG® Implants Material Stainless steel	C5302.3310	3.3 mm	33.1 mm
		C5302.4310	3.8 mm	
			4.3 mm	
	Holding sleeve for screw implants color-coded Material Titanium alloy	J5302.3300	3.3 mm	-
		J5302.3800	3.8 mm	
		J5302.4300	4.3 mm	
		J5302.5000	5.0 mm	
	Screwdriver hex, extra short, manuell/wrench Material Stainless steel	J5317.0510	-	14.5 mm
	Screwdriver hex, short, manual/wrench Material Stainless steel	J5317.0501	-	22.5 mm
	Screwdriver hex, long, manual/wrench Material Stainless steel	J5317.0502	-	30.3 mm

General surgical instruments

	Article	Art. No.	Dimension
	Screwdriver hex, short, ISO shaft Material Stainless steel	J5317.0504	18.0 mm
	Screwdriver hex, long, ISO shaft Material Stainless steel	J5317.0503	26.0 mm
	Manual screwdriver, hex without wrench head connection Material Stainless steel	J5317.0511	23.0 mm
	Cleaning needle for instruments with internal irrigation Material Stainless steel	J5002.0012	-
	Cleaning cannula for drills with internal irrigation Material Stainless steel	J5002.0020	-

SCREW-LINE

Osteotomy set


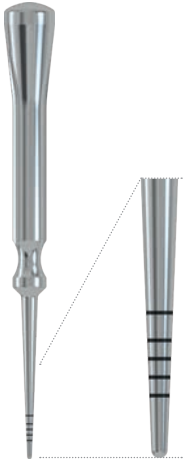
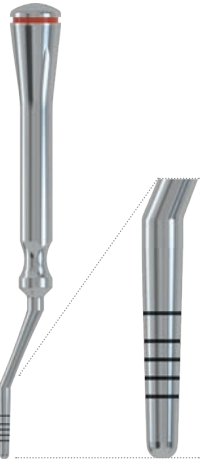
	Article	Art. No.	Ø
	<p>Osteotomy set CAMLOG®/CONOLOG® SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5418.0020</p>	<p>-</p>
	<p>Pre-Osteotome SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5417.2800*</p>	<p>1.7 – 2.8 mm</p>
	<p>Osteotome SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5418.3300* J5418.3800* J5418.4300* J5418.5000*</p>	<p>3.3 mm 3.8 mm 4.3 mm 5.0 mm</p>

Surgery


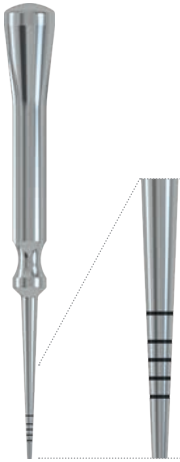
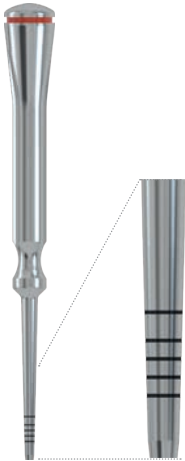
* These products are also included in the osteotomy set CAMLOG®/CONOLOG® SCREW-LINE straight convex.

SCREW-LINE

Osteotomy set

	Article	Art. No.	Ø
	<p>Osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled convex</p> <p>Material Stainless steel</p>	<p>J5418.0030</p>	<p>-</p>
	<p>Pre-Osteotome SCREW-LINE straight convex</p> <p>Material Stainless steel</p>	<p>J5417.2800*</p>	<p>1.7 – 2.8 mm</p>
	<p>Osteotome SCREW-LINE angled convex</p> <p>Material Stainless steel</p>	<p>J5418.3310* J5418.3810* J5418.4310* J5418.5010*</p>	<p>3.3 mm 3.8 mm 4.3 mm 5.0 mm</p>


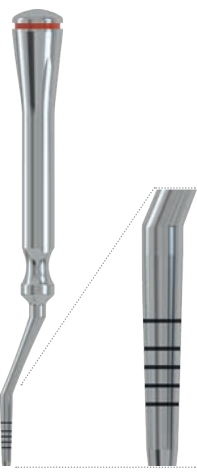
* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled convex.

	Article	Art. No.	Ø
	<p>Osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight concave</p> <p>Material Stainless steel</p>	J5420.0020	-
	<p>Pre-Osteotome SCREW-LINE straight concave</p> <p>Material Stainless steel</p>	J5419.2800*	1.7 – 2.8 mm
	<p>Osteotome SCREW-LINE straight concave</p> <p>Material Stainless steel</p>	J5420.3300*	3.3 mm
		J5420.3800*	3.8 mm
		J5420.4300*	4.3 mm
		J5420.5000*	5.0 mm

* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight concave.






SCREW-LINE

Osteotomy set

	Article	Art. No.	Ø
	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled concave Material Stainless steel	J5420.0030	-
	Pre-Osteotome SCREW-LINE straight concave Material Stainless steel	J5419.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE angled concave Material Stainless steel	J5420.3310*	3.3 mm
		J5420.3810*	3.8 mm
		J5420.4310*	4.3 mm
		J5420.5010*	5.0 mm






* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled concave.

ALTApin set



	Article	Art. No.
	<p>ALTApin set Membrane fixation system, resterilizable</p> <p>Material Plastic/Titanium alloy/Stainless steel</p>	M5600.0110
	<p>ALTApin tray (without content)</p> <p>Material Plastic</p>	M5600.0210
	<p>ALTApin applicator, straight inkl. aktivator</p> <p>Material Stainless steel</p>	M5100.0010*
	<p>ALTApin applicator, angled 90° inkl. aktivator</p> <p>Material Stainless steel</p>	M5100.0030
	<p>ALTApin applicator, straight, work element inkl. aktivator</p> <p>Material Stainless steel</p>	M5200.0010

* These products are included in the ALTApin set.


ALTApin set

	Article	Art. No.
	<p>ALTApin pricker</p> <p>Material Stainless steel</p>	M5100.0050*
	<p>ALTApin membrane fixator</p> <p>Material Stainless steel</p>	M5100.0070*
	<p>ALTApin surgery mallet</p> <p>Material Stainless steel/POM</p>	M5100.0100
	<p>ALTApin single patient drill, ISO shaft</p> <p>Material Stainless steel</p>	M5500.0050
	<p>ALTApin pricker, insert</p> <p>Material Stainless steel</p>	M5200.0055*




* These products are included in the ALTApin set.

	Article	Art. No.
	ALTApin magazine 7 titanium pins, sterile, 1 unit Material Titanium alloy	M1000.0050*
	ALTApin magazine 7 titanium pins, sterile, 3 units Material Titanium alloy	M1000.0100

Cover screws

	Article	Art. No.	Ø
	CONELOG® Implant cover screw Material Titanium alloy	C2019.3300	3.3 mm
		C2019.3800	3.8 mm
		C2019.4300	4.3 mm
		C2019.5000	5.0 mm

Healing caps

	Article	Art. No.	Ø	GH	G Ø
	CONELOG® Healing cap, cylindrical sterile Material Titanium alloy	C2015.3320	3.3 mm	2.0 mm	3.0 mm
		C2015.3340		4.0 mm	3.0 mm
		C2015.3820	3.8 mm	2.0 mm	3.5 mm
		C2015.3840		4.0 mm	3.5 mm
		C2015.3860**	6.0 mm	3.5 mm	
		C2015.4320	4.3 mm	2.0 mm	3.8 mm
		C2015.4340		4.0 mm	3.8 mm
		C2015.4360**	6.0 mm	3.8 mm	
		C2015.5020	5.0 mm	2.0 mm	4.5 mm
		C2015.5040		4.0 mm	4.5 mm
C2015.5060**	6.0 mm	4.5 mm			
	CONELOG® Healing cap, wide body sterile Material Titanium alloy	C2014.3340	3.3 mm	4.0 mm	4.8 mm
		C2014.3840	3.8 mm	4.0 mm	5.3 mm
		C2014.3860		6.0 mm	5.3 mm
		C2014.4340	4.3 mm	4.0 mm	5.8 mm
		C2014.4360		6.0 mm	5.8 mm
		C2014.5040	5.0 mm	4.0 mm	6.5 mm
C2014.5060	6.0 mm	6.5 mm			
	CONELOG® Healing cap, bottleneck sterile Material Titanium alloy	C2011.3340	3.3 mm	4.0 mm	3.3 mm
		C2011.3840	3.8 mm	4.0 mm	3.8 mm
		C2011.3860		6.0 mm	3.8 mm
		C2011.4340	4.3 mm	4.0 mm	4.0 mm
		C2011.4360		6.0 mm	4.0 mm
		C2011.5040	5.0 mm	4.0 mm	4.7 mm
C2011.5060	6.0 mm	4.7 mm			




* These products are included in the ALTApin set.

** suitable for bite registration








Impression taking

	Article	Art. No.	Ø
	CONELOG® Impression posts, open tray incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex) Material Titanium alloy	C2121.3300	3.3 mm
		C2121.3800	3.8 mm
		C2121.4300	4.3 mm
		C2121.5000	5.0 mm
	CONELOG® Impression posts, closed tray incl. impression cap, bite registration cap and fixing screw Material Titanium alloy/POM	C2110.3300	3.3 mm
		C2110.3800	3.8 mm
		C2110.4300	4.3 mm
		C2110.5000	5.0 mm
	Impression caps for impression post, closed tray (5 units) Material POM	J2111.3300	3.3 mm
		J2111.3800	3.8 mm
		J2111.4300	4.3 mm
		J2111.5000	5.0 mm

Bite registration

	Article	Art. No.	Ø
	CONELOG® Bite registration posts incl. fixing screw and bite registration cap Material Titanium alloy/POM	C2140.3300	3.3 mm
		C2140.3800	3.8 mm
		C2140.4300	4.3 mm
		C2140.5000	5.0 mm
	Bite registration caps (5 units) Material POM	J2112.3300	3.3 mm
		J2112.3800	3.8 mm
		J2112.4300	4.3 mm
		J2112.5000	5.0 mm

Fabrication of the plaster model

	Article	Art. No.	Ø
	CONELOG® Lab analog for cast models Material Titanium alloy	C3010.3300	3.3 mm
		C3010.3800	3.8 mm
		C3010.4300	4.3 mm
		C3010.5000	5.0 mm
	CONELOG® Implant analog for printed and cast models Material Titanium alloy	C3025.3300	3.3 mm
		C3025.3800	3.8 mm
		C3025.4300	4.3 mm
		C3025.5000	5.0 mm
	DIM Analog® for the CONELOG® Implant System for printed models, incl. thumbscrew Material Titanium alloy/Stainless steel	C3012.3300	3.3 mm
		C3012.4300	3.8 mm
			4.3 mm
		C3012.5000	5.0 mm



Manufacturer DIM Analog®: nt-trading GmbH & Co. KG, G.-Braun-Straße 18, 76187 Karlsruhe, Germany
 DIM Analog® is a registered trademark of nt-trading GmbH & Co. KG

Temporary restoration




	Article	Art. No.	Ø	GH
	CONELOG® Temporary abutment, crown, titanium alloy preparable, incl. abutment screw Material Titanium alloy	C2239.3300	3.3 mm*	-
		C2239.3800	3.8 mm	
		C2239.4300	4.3 mm	
		C2239.5000	5.0 mm	
	CONELOG® Temporary abutment, bridge, titanium alloy preparable, incl. abutment screw Material Titanium alloy	C2339.3300	3.3 mm	-
		C2339.3800	3.8 mm	
		C2339.4300	4.3 mm	
		C2339.5000	5.0 mm	

Esthomic® Abutments

Cemented crown and bridge restorations

	Article	Art. No.	Ø	GH
	CONELOG® Esthomic® Abutments, straight preparable, incl. abutment screw Material Titanium alloy	C2226.3815	3.8 mm	1.5 – 2.5 mm
		C2226.3830		3.0 – 4.5 mm
		C2226.4315	4.3 mm	1.5 – 2.5 mm
		C2226.4330		3.0 – 4.5 mm
		C2226.5015	5.0 mm	1.5 – 2.5 mm
		C2226.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, 15° angled, type A preparable, incl. abutment screw Material Titanium alloy	C2227.3815	3.8 mm	1.5 – 2.5 mm
		C2227.3830		3.0 – 4.5 mm
		C2227.4315	4.3 mm	1.5 – 2.5 mm
		C2227.4330		3.0 – 4.5 mm
		C2227.5015	5.0 mm	1.5 – 2.5 mm
		C2227.5030		3.0 – 4.5 mm





* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

	Article	Art. No.	Ø	GH
	CONELOG® Esthomic® Abutments, 15° angled, type B preparable, incl. abutment screw Material Titanium alloy	C2228.3815	3.8 mm	1.5 – 2.5 mm
		C2228.3830		3.0 – 4.5 mm
		C2228.4315	4.3 mm	1.5 – 2.5 mm
		C2228.4330		3.0 – 4.5 mm
		C2228.5015	5.0 mm	1.5 – 2.5 mm
		C2228.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, 20° angled, type A preparable, incl. abutment screw Material Titanium alloy	C2231.3815	3.8 mm	1.5 – 2.5 mm
		C2231.3830		3.0 – 4.5 mm
		C2231.4315	4.3 mm	1.5 – 2.5 mm
		C2231.4330		3.0 – 4.5 mm
		C2231.5015	5.0 mm	1.5 – 2.5 mm
		C2231.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, 20° angled, type B preparable, incl. abutment screw Material Titanium alloy	C2232.3815	3.8 mm	1.5 – 2.5 mm
		C2232.3830		3.0 – 4.5 mm
		C2232.4315	4.3 mm	1.5 – 2.5 mm
		C2232.4330		3.0 – 4.5 mm
		C2232.5015	5.0 mm	1.5 – 2.5 mm
		C2232.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, Inset preparable, incl. abutment screw Material Titanium alloy	C2235.3320	3.3 mm*	2.0 – 3.3 mm
		C2235.3820	3.8 mm	
		C2235.4320	4.3 mm	
		C2235.5020	5.0 mm	

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

CAD/CAM prosthetics

Crown, bridge and hybrid restorations







	Article	Art. No.	Ø	GH
	CONELOG® Titanium bases CAD/CAM, crown bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2242.3308	3.3 mm*	0.8 mm
		C2242.3808	3.8 mm	
		C2242.4308	4.3 mm	
		C2242.5008	5.0 mm	
	CONELOG® Titanium bases CAD/CAM, crown bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2242.3320	3.3 mm*	2.0 mm
		C2242.3820	3.8 mm	
		C2242.4320	4.3 mm	
		C2242.5020	5.0 mm	
	CONELOG® Titanium bases CAD/CAM, bridge bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2342.3308	3.3 mm	0.8 mm
		C2342.3808	3.8 mm	
		C2342.4308	4.3 mm	
		C2342.5008	5.0 mm	
	CONELOG® Titanium bases CAD/CAM, bridge bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2342.3320	3.3 mm	2.0 mm
		C2342.3820	3.8 mm	
		C2342.4320	4.3 mm	
		C2342.5020	5.0 mm	

The geometries of the CONELOG® Titanium bases CAD/CAM are available as a CAD library for leading dental CAD systems. The libraries are available for free download at: www.camlog.com/en/media-center/cad-libraries.

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® Products at your appropriate Camlog country representative.

	Article	Art. No.	Ø	Thread
 <p>11 mm</p>	CONELOG® Modeling aids for CAMLOG® Titanium bases CAD/CAM burn-out, for fabricating mesostructures and crowns Material POM	C2242.3302	3.3 mm	-
		C2242.3802	3.8 mm	
		C2242.4302	4.3 mm	
		C2242.5002	5.0 mm	
	CONELOG® Abutment screw for CONELOG® Titanium bases CAD/CAM dark purple anodized Material Titanium alloy	C4015.1601	3.3 mm	M 1.6
			3.8 mm	
	CONELOG® Lab screw for CONELOG® Titanium bases CAD/CAM brown partial anodized Material Titanium alloy	C4016.1601	3.3 mm	M 1.6
			3.8 mm	
	CONELOG® Lab screw for CONELOG® Titanium bases CAD/CAM brown partial anodized Material Titanium alloy	C4016.2001	4.3 mm	M 2.0
			5.0 mm	
 <p>10 mm</p>	CONELOG® Scanbodies* for optical, 3-dimensional localization of CONELOG® Implants in the mouth or CONELOG® Lab analogs in the working model, incl. abutment screw, sterile Not compatible with the CEREC and inLab systems from Sirona® Material PEEK	C2600.3310	3.3 mm	-
		C2600.4310	3.8 mm	
			4.3 mm	
 <p>10.2 mm</p>	CONELOG® ScanPosts for Sirona® Scanbody for digital recording of the CONELOG® Implant or lab analog position and for further processing in the Sirona® CEREC and inLab systems, incl. abutment screw Material Titanium alloy	C2620.3306	3.3 mm	-
		C2620.3806	3.8 mm	
		C2620.4306	4.3 mm	
		C2620.5006	5.0 mm	

* Please check whether the CONELOG® Scanbody is available in the CAD software used. CAD libraries for selected CONELOG® Prosthetic components are available for free download at: www.camlog.com/en/media-center/cad-libraries

Matching Sirona® Scanbodies size S for CONELOG® ScanPosts and CONELOG® Titanium base CAD/CAM crown with Ø 3.3/3.8/4.3 mm:

For Omnicam®: Article number 6431311

For Bluecam®: Article number 6431295

Matching Sirona® Scanbodies size L for CONELOG® ScanPosts and CONELOG® Titanium base CAD/CAM crown with Ø 5.0 mm:

For Omnicam®: Article number 6431329

For Bluecam®: Article number 6431303

Sirona® Scanbodies are available from Dentsply Sirona®.

CAM titanium blanks

Milling production process of individualized one-piece abutments and healing caps by CAD/CAM technology

	Article	Art. No.	Ø
	CONELOG® CAM titanium blank, type IAC* Ø 12 mm, length 12.5 mm (2 units), sent with 2 separate packed abutment screws Material Titanium alloy	C2411.3313	3.3 mm
		C2411.4313	3.8 mm
			4.3 mm
			5.0 mm
	CONELOG® CAM titanium blank, type ME** Ø 12 mm, length 20 mm (2 units), sent with 2 separate packed abutment screws Material Titanium alloy	C2421.3320	3.3 mm
		C2421.3820	3.8 mm
			4.3 mm
			5.0 mm

Accessories for CAM titanium blanks, type IAC

	Article	Art. No.	Ø
	CONELOG® Collet for CAM blank, type IAC* Ø 6 mm, length 17 mm, incl. 2 fixing screws for CAM blank, type IAC Material Stainless steel	C3720.3300	3.3 mm
		C3720.4300	3.8 mm
			4.3 mm
			5.0 mm

Type IAC*

For the milling process, the CAM titanium blank type IAC is fixated to the implant-abutment connection via the CONELOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.

Type ME**

For the milling process, the CAM titanium blank type ME is fixated with the front-facing groove of its cylindrical section via a milling holder for PreFace® Abutments from Medentika®. These milling holders are available for selected machines from the particular machine manufacturer.

The CAM titanium blanks require product specific CAM libraries which are available on request for selected CAM softwares from the software provider.


The geometries of the CONELOG® CAM Titanium Blanks are available as a CAD library for leading dental CAD systems. The libraries are available for free download at:

www.camlog.com/en/media-center/cad-libraries.

Medentika® and Preface® are registered trademarks of Medentika GmbH, D-Hügelsheim.


Universal abutments

Cemented crown and bridge restorations

	Article	Art. No.	Ø	Dimension
 <p>11 mm</p>	CONELOG® Universal abutments preparable, incl. abutment screw Material Titanium alloy	C2211.3300	3.3 mm*	-
		C2211.3800	3.8 mm	
		C2211.4300	4.3 mm	
		C2211.5000	5.0 mm	

Gold-plastic abutment






Cemented crown and bridge restorations

	Article	Art. No.	Ø	Noble metal weight
 <p>11.7 mm</p>	CONELOG® Gold-plastic abutment cast-on, incl. abutment screw Material Cast-on gold alloy/POM	C2246.3300	3.3 mm*	ca. 0.31 g
		C2246.3800	3.8 mm	ca. 0.36 g
		C2246.4300	4.3 mm	ca. 0.36 g
		C2246.5000	5.0 mm	ca. 0.55 g




* only for crown restorations in the region of the upper lateral and lower lateral and central incisors (Ø 3.3 mm not for double crown restorations)

Logfit® Prosthetic system

Cemented crown and bridge restorations












	Article	Art. No.	Ø	GH
	CONELOG® Logfit® Abutments incl. abutment screw Material Titanium alloy	C2550.3810	3.8 mm	1.0 mm
		C2550.3825		2.5 mm
		C2550.4310	4.3 mm	1.0 mm
		C2550.4325		2.5 mm
		C2550.5010	5.0 mm	1.0 mm
		C2550.5025		2.5 mm
	Logfit® Impression caps Material POM	J2551.4300	3.8 mm	-
		J2551.6000	4.3 mm	
			5.0 mm	
	Logfit® Analog Material Titanium alloy	J2552.4300	3.8 mm	-
			4.3 mm	
		J2552.6000	5.0 mm	
	Logfit® Plastic copings, for crowns (with rotation securing device) burn-out Material POM	J2553.4302	3.8 mm	-
			4.3 mm	
		J2553.6002	5.0 mm	
	Logfit® Plastic copings, for bridges (without rotation securing device) burn-out Material POM	J2553.4301	3.8 mm	-
			4.3 mm	
		J2553.6001	5.0 mm	

Occlusally screw-retained restorations

	Article	Art. No.	Typ	Ø	GH	PP Ø
	CONELOG® Bar abutment, straight sterile Material Titanium alloy	C2254.3310	-	3.3 mm	1.0 mm	4.3 mm
		C2254.3325			2.5 mm	
		C2254.3810		3.8 mm	1.0 mm	4.3 mm
		C2254.3825			2.5 mm	
		C2254.3840			4.0 mm	
		C2254.4310		4.3 mm	1.0 mm	4.3 mm
		C2254.4325			2.5 mm	
		C2254.4340			4.0 mm	
		C2254.5010		5.0 mm	1.0 mm	6.0 mm
		C2254.5025			2.5 mm	
C2254.5040	4.0 mm					
	CONELOG® Bar abutment, 17° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	C2256.3325	A	3.3 mm	2.5 mm	4.3 mm
		C2256.3340			4.0 mm	
		C2257.3325	B		2.5 mm	
		C2257.3340			4.0 mm	
		C2256.3825	A	3.8 mm	2.5 mm	4.3 mm
		C2256.3840			4.0 mm	
		C2257.3825	B		2.5 mm	
		C2257.3840			4.0 mm	
		C2256.4325	A	4.3 mm	2.5 mm	4.3 mm
		C2256.4340			4.0 mm	
		C2257.4325	B		2.5 mm	
		C2257.4340			4.0 mm	
		C2256.5025	A	5.0 mm	2.5 mm	6.0 mm
		C2256.5040			4.0 mm	
		C2257.5025	B		2.5 mm	
		C2257.5040			4.0 mm	
	CONELOG® Bar abutment, 30° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	C2258.3325	A	3.3 mm	2.5 mm	4.3 mm
		C2258.3340			4.0 mm	
		C2259.3325	B		2.5 mm	
		C2259.3340			4.0 mm	
		C2258.3825	A	3.8 mm	2.5 mm	4.3 mm
		C2258.3840			4.0 mm	
		C2259.3825	B		2.5 mm	
		C2259.3840			4.0 mm	
		C2258.4325	A	4.3 mm	2.5 mm	4.3 mm
		C2258.4340			4.0 mm	
		C2259.4325	B		2.5 mm	
		C2259.4340			4.0 mm	
		C2258.5035	A	5.0 mm	3.5 mm	6.0 mm
		C2258.5050			5.0 mm	
		C2259.5035	B		3.5 mm	
		C2259.5050			5.0 mm	











Type A and B see on page 6

Occlusally screw-retained restorations









	Article	Art. No.	Ø	Dimension
	Orientation gauge for COMFOUR® for Ø 2.0 mm pilot drill hole Material Nitinol	J3551.0001	-	-
	Aligning tool for angled bar abutments, for insertion post Material Stainless steel	J2269.0003*	-	17°
		J2269.0004*	-	30°
		J2269.0005**	-	17°
		J2269.0006**	-	30°
	Gingiva height indicator, straight Material Titanium alloy	J3550.3300	3.3 mm	-
		J3550.3800	3.8 mm	
		J3550.4300	4.3 mm	
		J3550.5000	5.0 mm	
	Driver for impression cap and healing cap for bar abutment Material Stainless steel	J5300.0027	3.3 mm 3.8 mm 4.3 mm	19.1 mm
		J5300.0028	5.0 mm	
	Healing cap for bar abutment partial light blue anodized, sterile Material Titanium alloy	J2029.4300	3.3 mm 3.8 mm 4.3 mm	-
		J2029.6000	5.0 mm	
	Impression cap, short, for bar abutment, closed tray (bridge/bar) partial light blue anodized, sterile Material Titanium alloy	J2129.4300	3.3 mm 3.8 mm 4.3 mm	6.5 mm
		J2129.6000	5.0 mm	7.0 mm
	Impression cap, long, for bar abutment, closed tray (bridge/bar) partial light blue anodized, sterile Material Titanium alloy	J2129.4310	3.3 mm 3.8 mm 4.3 mm	11.0 mm
		J2129.6010	5.0 mm	
	Bar lab analog for bar abutments Material Stainless steel	J3020.4300	3.3 mm 3.8 mm 4.3 mm	-
		J3020.6000	5.0 mm	
	Bar implant analog for bar abutments for printed and cast models Material Stainless steel	J3025.4300	3.3 mm 3.8 mm 4.3 mm	-
		J3025.6000	5.0 mm	
	Scanning cap for bar abutments incl. prosthetic screw, light blue anodized, sterile Material PEEK	J2610.4300	3.3 mm 3.8 mm 4.3 mm	-
		J2610.6000	5.0 mm	
	Titanium cap for bar abutment, for crown incl. prosthetic screw light blue anodized, sterile Material Titanium alloy	J2259.4301	3.3 mm 3.8 mm 4.3 mm	-
		J2259.6001	5.0 mm	

* only for use with CONELOG® Implants with Art. No. C1062.xxxx and C1063.xxxx.


** only for use with CONELOG® Implants with Art. No. C1064.xxxx and C1086.xxxx.

	Article	Art. No.	Ø			Dimension
	Titanium cap for bar abutment, for bridge incl. prosthetic screw light blue anodized, sterile	J2259.4302	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6002	5.0 mm			
	Titanium cap without retention for bar abutment, for bridge incl. prosthetic screw light blue anodized	J2259.4322	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6022	5.0 mm			
	Crown base for bar abutment burn-out	J2256.4306	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2256.6006	5.0 mm			
	Base for bar abutment burn-out	J2257.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2257.6001	5.0 mm			
	Base for bar abutment cast-on	J2263.4300	3.3 mm	3.8 mm	4.3 mm	ca. 0.48 g
	Material Cast-on gold alloy/POM	J2263.6000	5.0 mm			ca. 0.70 g
	Base for bar abutment solderable	J2258.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Solderable gold alloy	J2258.6000	5.0 mm			
	Base for bar abutment, titanium laser-weldable	J2262.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Titan Grade 4	J2262.6000	5.0 mm			
	Titanium bonding base for bar abutment Passive-Fit	J2260.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2260.6001	5.0 mm			
	Bar sleeve for titanium bonding base burn-out, Passive-Fit, incl. prosthetic screw for bar abutments, hex (only for fabrication of the cast framework in conjunction with bar sleeves for titanium bonding base Passive-Fit)	J2261.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2261.6001	5.0 mm			
	Polishing protection for caps and bases for bar abutment	J3021.4300	3.3 mm	3.8 mm	4.3 mm	Thread M 1.6
	Material Titanium alloy	J3021.6000	5.0 mm			Thread M 2.0




Occlusally screw-retained restorations

	Article	Art. No.	Ø			Thread
	Locator® Fixture for bar abutment	J2253.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy/TiN	J2253.6001	5.0 mm			
	CONELOG® Abutment screw with reduced head, hex, light blue anodized	C4004.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	C4004.2001	5.0 mm			M 2.0
	CONELOG® Lab screw reduced head, hex, partial light blue anodized	C4004.1600	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	C4004.2000	5.0 mm			M 2.0
	Prosthetic screw for bar abutments hex, light blue anodized (for final fixation of the restoration)	J4012.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4012.2001	5.0 mm			M 2.0
	Lab prosthetic screw for bar abutment hex, brown anodized	J4013.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4013.2001	5.0 mm			M 2.0
	Screw, hex, length 10 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1610	-			M 1.6
	Material Titanium alloy	J4012.2010				M 2.0
	Screw, hex, length 15 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1615	-			M 1.6
	Material Titanium alloy	J4012.2015				M 2.0
	Screw, hex, length 20 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1620	-			M 1.6
	Material Titanium alloy	J4012.2020				M 2.0

Lab screws may not be used on patients.

	Article	Art. No.	Ø	Thread
	Plastic screw for bar abutment hex, length 27 mm, sterile Material PEEK	J4009.1627	-	M 1.6
		J4009.2027		M 2.0

Ball abutment anchoring system

	Article	Art. No.	Ø	GH
	CONELOG® Ball abutment male part incl. stabilizing ring Material Titanium alloy/Plastic	C2249.3315	3.3 mm	1.5 mm
		C2249.3330		3.0 mm
		C2249.3815	3.8 mm	1.5 mm
		C2249.3830		3.0 mm
		C2249.3845	4.3 mm	4.5 mm
		C2249.4315		1.5 mm
		C2249.4330	5.0 mm	3.0 mm
		C2249.4345		4.5 mm
		C2249.5015	5.0 mm	1.5 mm
		C2249.5030		3.0 mm
C2249.5045	4.5 mm			
	Matrix CM Dalbo®-Plus for ball abutment, incl. lamella retention insert Material Titanium Grade 4/Gold alloy	05003503	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Lamella retention insert for matrix CM Dalbo®-Plus Material Gold alloy	05003504	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	




Dalbo®-Plus is a registered trademark of Cendres + Métaux SA, Biel, Switzerland.








Ball abutment anchoring system

	Article	Art. No.	Ø	GH
	Ball abutment analogs incl. stabilizing ring Material Brass/Plastic	C3015.3300	3.3 mm	-
			3.8 mm	
			4.3 mm	
		C3015.5000	5.0 mm	

Locator® Anchoring system


CONELOG® Locator R-Tx®

	Article	Art. No.	Ø	GH
	CONELOG® Locator R-Tx® Abutment incl. titanium housing with processing replacement male black, block-out spacer white and four different retention inserts Material Titanium alloy/Nylon	30805-01	3.3 mm	1.0 mm
		30805-02		2.0 mm
		30805-03		3.0 mm
		30805-04		4.0 mm
		30806-01	3.8 mm	1.0 mm
		30806-02		2.0 mm
		30806-03		3.0 mm
		30806-04		4.0 mm
		30806-05	4.3 mm	5.0 mm
		30807-01		1.0 mm
		30807-02		2.0 mm
		30807-03		3.0 mm
		30807-04		4.0 mm
		30807-05	5.0 mm	
		30808-01	5.0 mm	1.0 mm
		30808-02		2.0 mm
		30808-03		3.0 mm
30808-04	4.0 mm			
30808-05	5.0 mm			
	Locator R-Tx® Impression coping (4 units) Material Polyethylene	30017-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator R-Tx® Analog Ø 3.35 mm (4 units) Material Aluminum	30014-01	3.3 mm	-
			3.8 mm	
			4.3 mm	

	Article	Art. No.	Ø	GH
	Locator R-Tx® Analog Ø 5.0 mm (4 units) Material Aluminum	30016-01	5.0 mm	-
	Locator R-Tx® Titanium housing with processing insert black (4 units) Material Titanium alloy/Polyethylene	30013-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Processing insert black (4 units) Material Polyethylene	30012-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Processing spacer (4 units) Material Polyethylene	30018-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Retention insert gray, ZERO RETENTION (4 units) Material Nylon	30001-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Retention insert blue, LIGHT (4 units) Material Nylon	30002-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Retention insert pink, MEDIUM (4 units) Material Nylon	30003-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-




Locator® Anchoring system






CONELOG® Locator R-Tx®

	Article	Art. No.	Ø	GH
	Locator R-Tx® Retention insert white, STRONG (4 units) Material Nylon	30004-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

Locator® Anchoring system




CONELOG® Locator®

	Article	Art. No.	Ø	GH
	CONELOG® Locator® Abutment Material Titanium alloy/TiN	C2253.3310	3.3 mm	1.0 mm
		C2253.3320		2.0 mm
		C2253.3330		3.0 mm
		C2253.3340		4.0 mm
		C2253.3810	3.8 mm	1.0 mm
		C2253.3820		2.0 mm
		C2253.3830		3.0 mm
		C2253.3840		4.0 mm
		C2253.3850	5.0 mm	
		C2253.4310	4.3 mm	1.0 mm
		C2253.4320		2.0 mm
		C2253.4330		3.0 mm
		C2253.4340		4.0 mm
		C2253.4350	5.0 mm	
		C2253.5010	5.0 mm	1.0 mm
		C2253.5020		2.0 mm
C2253.5030	3.0 mm			
C2253.5040	4.0 mm			
C2253.5050	5.0 mm			
	Locator® Impression cap (4 units) Material Aluminum/Polyethylene	J2253.0200	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator® Analog (4 units) Material Aluminum	J2253.0340	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

	Article	Art. No.	Ø
	Locator® Male processing package (2 units) Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male clear 1 Replacement male pink 1 Replacement male blue Material Titanium alloy/Polyethylene/Teflon/Nylon	J2253.0102	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Male processing package for extended range (2 units) Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male green, 1 Replacement male orange, 1 Replacement male red Material Titanium alloy/Polyethylen/Teflon/Nylon	J2253.0112	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Block out spacer (20 units) Material Teflon	J2253.0401	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Processing replacement male (4 units) Material Polyethylen	J2253.0402	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male clear, STRONG, Div.: 0°-10° (4 units) Material Nylon	J2253.1005	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm

Locator® Anchoring system


CONELOG® Locator®

	Article	Art. No.	Ø
	Locator® Replacement male pink, MEDIUM, Div.: 0° – 10° (4 units) Material Nylon	J2253.1003	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male blue, LIGHT, Div.: 0° – 10° (4 units) Material Nylon	J2253.1002	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* green, STRONG, Div.: 10° – 20° (4 units) Material Nylon	J2253.2004	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* orange, MEDIUM, Div.: 10° – 20° (4 units) Material Nylon	J2253.2003	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* red, LIGHT, Div.: 10° – 20° (4 units) Material Nylon	J2253.2002	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* gray, NO RETENTION, Div.: 0° – 20° (4 units) Material Nylon	J2253.2000	3.8 mm
			4.3 mm
			5.0 mm



* not permitted for implant Ø 3.3 mm

Manufacturer Locator®: Zest Anchors, 2875 Loker Avenue East, Carlsbad, California 92010, USA
Locator® and Locator R-Tx® are registered trademarks of Zest Anchors

Double crown restoration

	Article	Art. No.	Ø
 <p>11 mm</p>	CONELOG® Universal abutments for double crown restorations preparable, incl. abutment screw Material Titanium alloy	C2211.3800	3.8 mm
		C2211.4300	4.3 mm
		C2211.5000	5.0 mm
 <p>12 mm</p>	CONELOG® Telescope abutments for double crown restorations preparable, incl. abutment screw Material Titanium alloy	C2212.3800	3.8 mm
		C2212.4300	4.3 mm
		C2212.5000	5.0 mm

Accessories for abutments

	Article	Art. No.	Ø	Thread
	CONELOG® Abutment screw, hex for definitive screw retention of abutments into the implant Material Titanium alloy	C4005.1601	3.3 mm	M 1.6
			3.8 mm	
		C4005.2001	4.3 mm	5.0 mm
	CONELOG® Lab screw, hex for the fixation of abutments on the working model, brown anodized Material Titanium alloy	C4006.1601	3.3 mm	M 1.6
			3.8 mm	
		C4006.2001	4.3 mm	5.0 mm







Lab screws may not be used on patients.





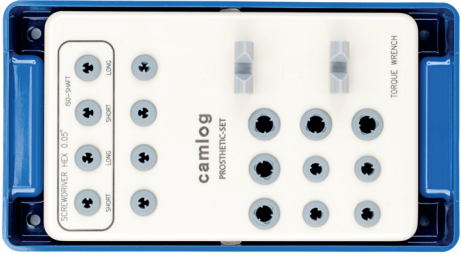


Prosthetic instruments

	Article	Art. No.	L
	<p>Torque wrench with continuous torque adjustment until maximal 30 Ncm</p> <p>Material Stainless steel</p>	J5320.1030	-
	<p>Driver for ball abutment, manual/wrench</p> <p>Material Stainless steel</p>	J5300.0011	18.3 mm
	<p>Screwdriver Activator for ball abutment matrix CM Dalbo®-Plus</p> <p>Material Stainless steel</p>	07000389	-
	<p>Driver for straight bar abutment, short Ø 3.3/3.8/4.3 mm</p> <p>Material Stainless steel</p>	J5300.0020	18.6 mm
	<p>Driver for straight bar abutment, short Ø 5.0 mm</p> <p>Material Stainless steel</p>	J5300.0025	18.6 mm





	Article	Art. No.	L
	<p>Driver for straight bar abutment, long Ø 3.3/3.8/4.3 mm</p> <p>Material Stainless steel</p>	J5300.0021	28.0 mm
	<p>Driver for impression cap and healing cap for bar abutment Ø 3.3/3.8/4.3 mm</p> <p>Material Stainless steel</p>	J5300.0027	19.1 mm
	<p>Driver for impression cap and healing cap for bar abutment Ø 5.0 mm</p> <p>Material Stainless steel</p>	J5300.0028	19.1 mm
	<p>Driver for Locator®, manual/wrench</p> <p>Material Stainless steel</p>	J2253.0001	24.3 mm
	<p>Locator® Instrument threepart</p> <p>Material Stainless steel</p>	J2253.0002	83.0 mm
	<p>Locator® Abutment holder sleeve for golden component of the Locator® Instrument (4 units)</p> <p>Material Polysulfone</p>	08394	-
	<p>Locator® Angle measurement guide</p> <p>Material Stainless steel</p>	J2253.0003	-
	<p>Locator® Parallel post (4 units)</p> <p>Material Polyethylene</p>	J2253.0004	-

Prosthetic instruments


	Article	Art. No.	L
	<p>Locator R-Tx® Retention insert tool with plastic grip</p> <p>Material Stainless steel</p>	30021-01	
	<p>Prosthetic set Content:</p> <ul style="list-style-type: none"> - J5320.1030 Torque wrench - J5317.0501 Screwdriver, hex, short, manual/wrench - J5317.0502 Screwdriver, hex, long, manual/wrench - J5317.0504 Screwdriver, hex, short, ISO shaft - J5317.0503 Screwdriver, hex, long, ISO shaft 	J5330.8600	197 x 108 x 54 mm
	<p>Prosthetic tray (without content)</p> <p>Material Plastic</p>	J5330.8500	197 x 108 x 54 mm
	<p>Prosthetic tray universal (without content) resterilizable</p> <p>Material Radel®/Silicone</p>	J5330.8700	162 x 73 x 29 mm
	<p>Screwdriver Hex, extra short, manual/wrench</p> <p>Material Stainless steel</p>	J5317.0510	14.5 mm
	<p>Screwdriver Hex, short, manual/wrench</p> <p>Material Stainless steel</p>	J5317.0501	22.5 mm

	Article	Art. No.	Ø	Dimension
	Screwdriver Hex, long, manual/wrench Material Stainless steel	J5317.0502	-	30.3 mm
	Screwdriver Hex, short, ISO shaft Material Stainless steel	J5317.0504	-	18.0 mm
	Screwdriver Hex, long, ISO shaft Material Stainless steel	J5317.0503	-	26.0 mm
	Manual screwdriver Hex, without wrench head connection Material Stainless steel	J5317.0511	-	23.0 mm
	Handle for CAMLOG®/CONELOG® Implant analog Material Stainless steel	J3025.0010	3.3 mm	-
		J3025.0015	5.0 mm	
	CONELOG® Disconnector for CONELOG® Abutments, short Material Stainless steel	C5300.1601	3.3 mm	Thread M 1.6
			3.8 mm	
			4.3 mm	
		C5300.2001	5.0 mm	Thread M 2.0
	CONELOG® Disconnector for CONELOG® Abutments, long Material Stainless steel	C5300.1603	3.3 mm	Thread M 1.6
			3.8 mm	
			4.3 mm	
		C5300.2003	5.0 mm	Thread M 2.0

Instruments for dental technicians

	Article	Art. No.	Ø
	Universal holder incl. 2 CONELOG® Lab screws, hex, and 1 CONELOG® Abutment collet each for Ø 3.3/3.8/4.3/5.0 mm Material Stainless steel/Titanium alloy	C3709.0010	-
	Universal holder Material Stainless steel	J3709.0015	-
	CONELOG® Abutment collets for universal holder, for grinding CAMLOG® Abutments Material Titanium alloy	C3709.3300	3.3 mm
		C3709.3800	3.8 mm
		C3709.4300	4.3 mm
		C3709.5000	5.0 mm
	Reworking reamer, for base for bar abutment plane surface, burn-out Material Stainless steel/Brass	J3711.0010	3.3 mm
			3.8 mm
		J3711.0015	4.3 mm
			5.0 mm
	Reworking reamer, for base for bar abutment screw seat, burn-out Material Stainless steel/Brass	J3711.0020	3.3 mm
			3.8 mm
		J3711.0025	4.3 mm
			5.0 mm



Selection abutments

	Article	Art. No.
	CONELOG® Selection abutment kit (Content: 2 units each, according table below)	C8011.1000

Content: CONELOG® Selection abutment kit					
Article	Material	Ø			GH
CONELOG® Esthomic® Selection abutment, straight*	POM	3.8 mm	4.3 mm	5.0 mm	1.5 - 2.5 mm
CONELOG® Esthomic® Selection abutment, 15° angled, type A*					3.0 - 4.5 mm
CONELOG® Esthomic® Selection abutment, 15° angled, type B*					1.5 - 2.5 mm
CONELOG® Esthomic® Selection abutment, 20° angled, type A*					
CONELOG® Esthomic® Selection abutment, 20° angled, type B*					





Attention, do not use selection abutments on patients!

* These products are not available singly.





Implants for practice



	Article	Art. No.	Ø	L
	CONELOG® PROGRESSIVE-LINE Implant for practice incl. snap-in insertion post and cover screw, yellow anodized Material Titanium alloy	C1901.3813	3.8 mm	13 mm
	CONELOG® PROGRESSIVE-LINE Implant for practice incl. snap-in insertion post and cover screw, red anodized Material Titanium alloy	C1901.4313	4.3 mm	
	CONELOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, yellow anodized Material Titanium alloy	C1069.3813	3.8 mm	13 mm
	CONELOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, red anodized Material Titanium alloy	C1069.4313	4.3 mm	

Attention, do not use implants for practice on patients!

Demonstration models



	Article	Art. No.
	<p>CONELOG® Demonstration model, acrylic glass upper jaw, 4 CONELOG® SCREW-LINE Implants, 4 x Ø 4.3 mm</p> <p>Material Acrylic glass/Titanium</p>	C8070.1020
	<p>CONELOG® Demonstration model, acrylic glass lower jaw, 4 CONELOG® SCREW-LINE Implants, 4 x Ø 4.3 mm</p> <p>Material Acrylic glass/Titanium</p>	C8050.1040
	<p>Edentulous mandible incl. mounting plate</p> <p>Material Plastic</p>	J8070.2050

Macro models

















	Article	Art. No.
	<p>CONELOG® PROGRESSIVE-LINE Macro model Scale 3:1</p> <p>Content: 1 CONELOG® PROGRESSIVE-LINE Implant 1 CONELOG® Esthomic® Abutment, straight 1 CONELOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic socket</p> <p>Material Plastic/Stainless steel</p>	C8010.1400
	<p>CONELOG® SCREW-LINE Macro model Scale 3:1</p> <p>Content: 1 CONELOG® SCREW-LINE Implant 1 CONELOG® Esthomic® Abutment, straight 1 CONELOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic socket</p> <p>Material Plastic/Stainless steel</p>	C8010.1010












Literature

	Article	Art. No.
	<p>Patient brochure Questions and answers to dental implants</p>	-
	<p>COMFOUR® Patient brochure Bridge instead of dentures – dental prosthesis with feel-good factor</p>	-
	<p>Implant pass Patient-specific documentation of implant restoration Packaging units: 10 units</p>	-
	<p>Patient advice sheets Set á 5 sheets, A4</p>	-
	<p>Presentation folder A4, laminated</p>	-

	Article	Art. No.
	<p>Poster Format: 50 x 70 cm</p>	<p>-</p>
	<p>Appointment pad 50 sheets/pad, A7 Packaging units: 5 units</p>	<p>-</p>

Indication overview



Single tooth restoration		Bridge restoration
Cemented	Screwed	Cemented
	 <p>Temporary abutment, crown, titanium alloy</p>	
 <p>Esthomic® Abutments</p>		 <p>Esthomic® Abutments</p>
	 <p>Bar abutments</p>	
 <p>Titanium bases CAD/CAM, crown</p>	 <p>Titanium bases CAD/CAM, crown</p>	 <p>Titanium bases CAD/CAM, bridge</p>
 <p>Logfit® Abutment</p>		 <p>Logfit® Abutment</p>
  <p>Universal abutment CAM titanium blank</p>		  <p>Universal abutment CAM titanium blank</p>
 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>



Bridge restoration	Hybrid restoration
Screwed	Removable (full denture)
 <p>Temporary abutment, bridge, titanium alloy</p>	
 <p>Bar abutments</p>	 <p>Bar abutments</p>
 <p>Titanium bases CAD/CAM, bridge</p>	
	 <p>Locator® Anchoring system</p>
	 <p>Ball abutment</p>
Double crown restoration	  <p>Universal abutment CAM titanium blank</p>
	 <p>Telescope abutment</p>
	 <p>Gold-plastic abutment</p>
	 <p>Titanium bases CAD/CAM, crown</p>

Auxiliary information






Implant overview

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No. A Ø				L
 <p>CONELOG® PROGRESSIVE-LINE Implant, Promote® plus with screw-mounted insertion post</p>	-	C1085.3807 A Ø 3.0 mm	C1085.4307 A Ø 3.0 mm	C1085.5007 A Ø 3.5 mm	7 mm	
	C1085.3309 A Ø 2.2 mm	C1085.3809 A Ø 3.0 mm	C1085.4309 A Ø 3.0 mm	C1085.5009 A Ø 3.5 mm	9 mm	
	C1085.3311 A Ø 2.2 mm	C1085.3811 A Ø 2.7 mm	C1085.4311 A Ø 2.7 mm	C1085.5011 A Ø 3.2 mm	11 mm	
	C1085.3313 A Ø 2.2 mm	C1085.3813 A Ø 2.7 mm	C1085.4313 A Ø 2.7 mm	C1085.5013 A Ø 3.2 mm	13 mm	
	C1085.3316 A Ø 2.2 mm	C1085.3816 A Ø 2.7 mm	C1085.4316 A Ø 2.7 mm	C1085.5016 A Ø 3.2 mm	16 mm	
 <p>CONELOG® PROGRESSIVE-LINE Implant, Promote® plus with snap-in insertion post</p>	-	C1086.3807 A Ø 3.0 mm	C1086.4307 A Ø 3.0 mm	C1086.5007 A Ø 3.5 mm	7 mm	
	C1086.3309 A Ø 2.2 mm	C1086.3809 A Ø 3.0 mm	C1086.4309 A Ø 3.0 mm	C1086.5009 A Ø 3.5 mm	9 mm	
	C1086.3311 A Ø 2.2 mm	C1086.3811 A Ø 2.7 mm	C1086.4311 A Ø 2.7 mm	C1086.5011 A Ø 3.2 mm	11 mm	
	C1086.3313 A Ø 2.2 mm	C1086.3813 A Ø 2.7 mm	C1086.4313 A Ø 2.7 mm	C1086.5013 A Ø 3.2 mm	13 mm	
	C1086.3316 A Ø 2.2 mm	C1086.3816 A Ø 2.7 mm	C1086.4316 A Ø 2.7 mm	C1086.5016 A Ø 3.2 mm	16 mm	


		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		A Ø 2.7 mm	A Ø 3.5 mm	A Ø 3.9 mm	A Ø 4.6 mm	
Article		Art. No.				L
 <p>CONELOG® SCREW-LINE Implant, Promote® plus with snap-in insertion post</p>	-	C1066.3807	C1066.4307	C1066.5007	7 mm	
	C1066.3309	C1066.3809	C1066.4309	C1066.5009	9 mm	
	C1066.3311	C1066.3811	C1066.4311	C1066.5011	11 mm	
	C1066.3313	C1066.3813	C1066.4313	C1066.5013	13 mm	
	C1066.3316	C1066.3816	C1066.4316	C1066.5016	16 mm	
 <p>CONELOG® SCREW-LINE Implant, Promote® plus with screw-mounted insertion post</p>	-	C1065.3807	C1065.4307	C1065.5007	7 mm	
	C1065.3309	C1065.3809	C1065.4309	C1065.5009	9 mm	
	C1065.3311	C1065.3811	C1065.4311	C1065.5011	11 mm	
	C1065.3313	C1065.3813	C1065.4313	C1065.5013	13 mm	
	C1065.3316	C1065.3816	C1065.4316	C1065.5016	16 mm	

Prosthetics overview




Impression taking

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Impression posts, open tray	C2121.3300	C2121.3800	C2121.4300	C2121.5000	-
	CONELOG® Impression posts, closed tray	C2110.3300	C2110.3800	C2110.4300	C2110.5000	-
	Impression caps for impression post, closed tray	J2111.3300	J2111.3800	J2111.4300	J2111.5000	-








Bite registration

	CONELOG® Bite registration posts incl. fixing screw and bite registration cap	C2140.3300	C2140.3800	C2140.4300	C2140.5000	-
---	--	------------	------------	------------	------------	---

Fabrication of the plaster model

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Lab analogs, for cast models	C3010.3300	C3010.3800	C3010.4300	C3010.5000	-
	CONELOG® Implant analog, for printed and cast models	C3025.3300	C3025.3800	C3025.4300	C3025.5000	-
	DIM Analog® for printed models, for the CONELOG® Implant System	C3012.3300	C3012.4300	C3012.4300	C3012.5000	-

Abutments for crown and bridge restoration















	CONELOG® Temporary abutments, crown, titanium alloy	C2239.3300	C2239.3800	C2239.4300	C2239.5000	-
	CONELOG® Temporary abutments, bridge, titanium alloy	C2339.3300	C2339.3800	C2339.4300	C2339.5000	-
	CONELOG® Esthomic® Abutments, straight	-	C2226.3815	C2226.4315	C2226.5015	1.5 - 2.5
			C2226.3830	C2226.4330	C2226.5030	3.0 - 4.5
	CONELOG® Esthomic® Abutments, 15° angled, type A	-	C2227.3815	C2227.4315	C2227.5015	1.5 - 2.5
			C2227.3830	C2227.4330	C2227.5030	3.0 - 4.5
	CONELOG® Esthomic® Abutments, 15° angled, type B	-	C2228.3815	C2228.4315	C2228.5015	1.5 - 2.5
			C2228.3830	C2228.4330	C2228.5030	3.0 - 4.5
	CONELOG® Esthomic® Abutments, 20° angled, type A	-	C2231.3815	C2231.4315	C2231.5015	1.5 - 2.5
			C2231.3830	C2231.4330	C2231.5030	3.0 - 4.5
	CONELOG® Esthomic® Abutments, 20° angled, type B	-	C2232.3815	C2232.4315	C2232.5015	1.5 - 2.5
			C2232.3830	C2232.4330	C2232.5030	3.0 - 4.5

Prosthetics overview

Abutments for crown and bridge restorations






		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Esthomic® Abutments Inset	C2235.3320	C2235.3820	C2235.4320	C2235.5020	2.0 – 3.3 mm
	CONELOG® Universal abutments	C2211.3300	C2211.3800	C2211.4300	C2211.5000	-
	CONELOG® Gold-plastic abutments	C2246.3300	C2246.3800	C2246.4300	C2246.5000	-
	CONELOG® Titanium bases CAD/CAM, crown	C2242.3308	C2242.3808	C2242.4308	C2242.5008	0.8 mm
		C2242.3320	C2242.3820	C2242.4320	C2242.5020	2.0 mm
	CONELOG® Titanium bases CAD/CAM, bridge	C2342.3308	C2342.3808	C2342.4308	C2342.5008	0.8 mm
		C2342.3320	C2342.3820	C2342.4320	C2342.5020	2.0 mm
	CONELOG® Logfit® Abutments	-	C2550.3810	C2550.4310	C2550.5010	1.0 mm
		-	C2550.3825	C2550.4325	C2550.5025	2.5 mm
	Logfit® Impression caps	-	J2551.4300	J2551.4300	J2551.6000	-
	Logfit® Analogs	-	J2552.4300	J2552.4300	J2552.6000	-
	Logfit® Plastic copings, for crowns	-	J2553.4302	J2553.4302	J2553.6002	-
	Logfit® Plastic copings, for bridges	-	J2553.4301	J2553.4301	J2553.6001	-

COMFOUR® Abutments for crown, bridge and hybrid restorations














		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Bar abutment, straight	C2254.3310	C2254.3810	C2254.4310	C2254.5010	1.0 mm
		C2254.3325	C2254.3825	C2254.4325	C2254.5025	2.5 mm
		-	C2254.3840	C2254.4340	C2254.5040	4.0 mm
	CONELOG® Bar abutment, 17° angled, type A	C2256.3325	C2256.3825	C2256.4325	C2256.5025	2.5 mm
		C2256.3340	C2256.3840	C2256.4340	C2256.5040	4.0 mm
	CONELOG® Bar abutment, 17° angled, type B	C2257.3325	C2257.3825	C2257.4325	C2257.5025	2.5 mm
		C2257.3340	C2257.3840	C2257.4340	C2257.5040	4.0 mm
	CONELOG® Bar abutment, 30° angled, Type A	C2258.3325	C2258.3825	C2258.4325	C2258.5035*	2.5 mm/ 3.5 mm*
		C2258.3340	C2258.3840	C2258.4340	C2258.5050*	4.0 mm/ 5.0 mm*
	CONELOG® Bar abutment, 30° angled, Type B	C2259.3325	C2259.3825	C2259.4325	C2259.5035*	2.5 mm/ 3.5 mm*
		C2259.3340	C2259.3840	C2259.4340	C2259.5050*	4.0 mm/ 5.0 mm*
	Healing cap for bar abutment	J2029.4300	J2029.4300	J2029.4300	J2029.6000	-
	Impression cap, short, for bar abutment, closed tray	J2129.4300	J2129.4300	J2129.4300	J2129.6000	-
	Impression cap, long, for bar abutment, closed tray (bridge/bar)	J2129.4310	J2129.4310	J2129.4310	J2129.6010	-
	Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-
	Titanium cap for bar abutment, for crown	J2259.4301	J2259.4301	J2259.4301	J2259.6001	-
	Titanium cap for bar abutment, for bridge	J2259.4302	J2259.4302	J2259.4302	J2259.6002	-
	Titanium cap without retention for bar abutment, for bridge	J2259.4322	J2259.4322	J2259.4322	J2259.6022	-
	Crown base for bar abutment, burn-out	J2256.4306	J2256.4306	J2256.4306	J2256.6006	-
	Base for bar abutment, burn-out	J2257.4301	J2257.4301	J2257.4301	J2257.6001	-
	Base for bar abutment, cast-on	J2263.4300	J2263.4300	J2263.4300	J2263.6000	-








Prosthetics overview

COMFOUR® Abutments for crown, bridge and hybrid restorations






		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	Base for bar abutment, solderable	J2258.4300	J2258.4300	J2258.4300	J2258.6000	-
	Base for bar abutment, titanium, laser-weldable	J2262.4300	J2262.4300	J2262.4300	J2262.6000	-
	Titanium bonding base for bar abutment, Passive-Fit	J2260.4301	J2260.4301	J2260.4301	J2260.6001	-
	Sleeve for titanium bonding base, burn-out, Passive-Fit	J2261.4301	J2261.4301	J2261.4301	J2261.6001	-
	Locator® Fixture for bar abutment	J2253.4301	J2253.4301	J2253.4301	J2253.6001	-

Hybrid restoration

	CONELOG® Ball abutment, male part	C2249.3315	C2249.3815	C2249.4315	C2249.5015	1.5 mm
		C2249.3330	C2249.3830	C2249.4330	C2249.5030	3.0 mm
		-	C2249.3845	C2249.4345	C2249.5045	4.5 mm
	Matrix CM Dalbo®-Plus	05003503	05003503	05003503	05003503	-
	Ball abutment analog	C3015.3300	C3015.3300	C3015.3300	C3015.5000	-
	CONELOG® Locator R-Tx® Abutment	30805-01	30806-01	30807-01	30808-01	1.0 mm
		30805-02	30806-02	30807-02	30808-02	2.0 mm
		30805-03	30806-03	30807-03	30808-03	3.0 mm
		30805-04	30806-04	30807-04	30808-04	4.0 mm
		-	30806-05	30807-05	30808-05	5.0 mm
	Locator R-Tx® Impression coping	30017-01	30017-01	30017-01	30017-01	-
	Locator R-Tx® Analog	30014-01	30014-01	30014-01	30016-01	-
	Locator R-Tx® Titanium housing	30013-01	30013-01	30013-01	30013-01	-
	Locator R-Tx® Processing insert	30012-01	30012-01	30012-01	30012-01	-
	Locator R-Tx® Processing spacer	30018-01	30018-01	30018-01	30018-01	-
	Locator R-Tx® Retention insert gray, ZERO RETENTION	30001-01	30001-01	30001-01	30001-01	-
	Locator R-Tx® Retention insert blue, LIGHT	30002-01	30002-01	30002-01	30002-01	-
	Locator R-Tx® Retention insert pink, MEDIUM	30003-01	30003-01	30003-01	30003-01	-
	Locator R-Tx® Retention insert white, STRONG	30004-01	30004-01	30004-01	30004-01	-

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Locator® Abutment	C2253.3310	C2253.3810	C2253.4310	C2253.5010	1.0 mm
		C2253.3320	C2253.3820	C2253.4320	C2253.5020	2.0 mm
		C2253.3330	C2253.3830	C2253.4330	C2253.5030	3.0 mm
		C2253.3340	C2253.3840	C2253.4340	C2253.5040	4.0 mm
		-	C2253.3850	C2253.4350	C2253.5050	5.0 mm
	Locator® Impression cap	J2253.0200	J2253.0200	J2253.0200	J2253.0200	-
	Locator® Analog	J2253.0340	J2253.0340	J2253.0340	J2253.0340	-
	Locator® Male processing package	J2253.0102	J2253.0102	J2253.0102	J2253.0102	-
	Locator® Male processing package for extended range	-	J2253.0112	J2253.0112	J2253.0112	-
	CONELOG® Universal abutment	-	C2211.3800	C2211.4300	C2211.5000	-
	CONELOG® Telescope abutment	-	C2212.3800	C2212.4300	C2212.5000	-

CAD/CAM prosthetics





















	CONELOG® Scanbodies	C2600.3310	C2600.4310	C2600.4310	C2600.5010	-
	CONELOG® ScanPost for Sirona® Scanbody	C2620.3306	C2620.3806	C2620.4306	C2620.5006	-
	CONELOG® CAM titanium blank, type IAC	C2411.3313	C2411.4313	C2411.4313	C2411.5013	-
	CONELOG® CAM titanium blank, type ME	C2421.3320	C2421.3820	C2421.4320	C2421.5020	-
	Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-

DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® Products at your appropriate Camlog country representative.

Screw overview Abutment and prosthetic screws – intraoral use

Implant-Abutment connection






	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		M 1.6		M 2.0	
Article	CONELOG® Abutment screw				Tightening torque
 <p>Scanbody ScanPost for Sirona® Scanbody</p>					tightened by hand**
 <p>Temporary abutments titanium, crown and bridge</p>					
 <p>Esthomic® Abutments</p>	8.9 mm		8.9 mm		20 Ncm*
<p>Universal abutment</p> 	 C4005.1601		 C4005.2001		
 <p>Telescope abutment</p>					
 <p>Gold-plastic abutment</p>					
 <p>Logfit® Abutment</p>					
 <p>Vario SR abutments, 20° und 30° angled</p>					
 <p>CONELOG® CAM titanium blank, type IAC and ME</p>					
CONELOG® Abutment screws for titanium bases CAD/CAM, dark purple anodized					
 <p>Titanium bases CAD/CAM, crown and bridge</p>	8.9 mm		8.9 mm		20 Ncm*
	 C4015.1601		 C4015.2001		
CONELOG® Vario SR abutment screws					
 <p>Vario SR abutment, straight</p>	10.6 mm		10.6 mm		20 Ncm*
	 C4007.1600		 C4007.2000		
CONELOG® Abutment screws with reduced head, light blue anodized					
 <p>COMFOUR® Bar abutments, 17° and 30° angled</p>	7.8 mm		7.8 mm		20 Ncm*
	 C4004.1601		 C4004.2001		

* with torque wrench J5320.1030

** Optional for temporary abutments titanium: torque after completed healing phase 20 Ncm.













All screws must be retightened with the corresponding torque after at least 5 minutes!

Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		M 1.6		M 2.0		
Article		Prosthetic screws for bar abutments, light blue anodized				Tightening torque
 <p>COMFOUR® Bar abutments, 17° and 30° angled</p>	3.6 mm  J4012.1601		3.8 mm  J4012.2001		15 Ncm*	
	Vario SR prosthetic screw, yellow anodized					
 <p>Vario SR abutments, straight, 20° and 30° angled</p>	4 mm  J4005.2004				15 Ncm*	

Auxiliary screws Intra- and extraoral use

Abutment-Prosthetic connection





















		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		M 1.6		M 2.0		
Article		Prosthetic screws for bar abutments, light blue anodized				Tightening torque
 <p>Scanning cap for bar abutments</p>	3.6 mm  J4012.1601		3.8 mm  J4012.2001		tightened by hand	
Screws for bar abutments, for impression taking open tray and for soldering, light blue anodized						
 <p>COMFOUR® Bar abutments, straight, 17° and 30° angled</p>	12 mm  J4012.1610		12.2 mm  J4012.2010		tightened by hand	
	17 mm  J4012.1615		17.2 mm  J4012.2015			
	22 mm  J4012.1620		22.2 mm  J4012.2020			
	Plastic screws for bar abutment, as fixation and bonding aid, beige					
		29 mm  J4009.1627		29.2 mm  J4009.2027		tightened by hand

* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

Screw overview Lab screws – extraoral use

Lab analog-Abutment connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		M 1.6		M 2.0	
Article	CONELOG® Lab screws*, brown anodized				Tightening torque
 <p>Scanbody ScanPost for Sirona® Scanbody</p>					tightened by hand
 <p>Temporary abutments titanium, crown and bridge</p>					
 <p>Esthomic® Abutments</p>	 8.9 mm		 8.9 mm		
 <p>Universal abutment Telescope abutment Gold-plastic abutment</p>	C4006.1601		C4006.2001		
 <p>Vario SR abutments, 20° and 30° angled</p>					
 <p>CONELOG® CAM titanium blank, type IAC and ME</p>					
CONELOG® Lab screws for titanium bases CAD/CAM*, brown anodized					
 <p>Titanium bases CAD/CAM, crown and bridge</p>	 8.9 mm C4016.1601		 8.9 mm C4016.2001		tightened by hand
CONELOG® Bonding aids**					
 <p>Titanium bases CAD/CAM, crown and bridge</p>	 26 mm		 26 mm		tightened by hand
CONELOG® Vario SR lab screws*, brown anodized					
 <p>Vario SR abutment, straight</p>	 10.6 mm C4008.1600		 10.6 mm C4008.2000		tightened by hand
CONELOG® Lab screws with reduced head*, light blue partially anodized					
 <p>COMFOUR® Bar abutments, 17° and 30° angled</p>	 7.8 mm C4004.1600		 7.8 mm C4004.2000		tightened by hand

* Lab screws may not be used on patients.













** not available singly, are included in the packaging of the titanium base CAD/CAM.

Abutment-Prosthetic connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M 1.6		M 2.0		
	Lab prosthetic screws for bar abutments*, brown anodized				Tightening torque
	Scanning cap for bar abutments				
	COMFOUR® Bar abutment, 17° and 30° angled		3.6 mm  J4013.1601	3.8 mm  J4013.2001	tightened by hand
	Bar lab analog for bar abutments				
Vario SR prosthetic screw, yellow anodized					
	Vario SR abutments, straight, 20° and 30° angled		4 mm  J4005.2004		tightened by hand
	Vario SR analog				
Prosthetic screw for bar abutments*, for fabrication of the wax up on the bar sleeve for titanium bonding base, Passive-Fit, on the bar lab analog					
	Titanium bonding base for bar abutments and bar sleeve for titanium bonding base, burn-out, Passive-Fit		5.5 mm  J4005.1602	5.5 mm  J4005.2002	tightened by hand

* Lab screws may not be used on patients.































Overview Tightening torque

Article	Instrument	Tightening torque
 <p>Implant cover screw</p>		
 <p>Healing caps cylindrical, wide body, bottleneck</p>		
 <p>Impression posts Bite registration post</p>		tightened by hand**
 <p>Lab screws Lab screws with reduced head</p>		
 <p>Temporary abutments titanium, crown and bridge</p>		
 <p>Abutment screws Abutment screws with reduced head</p>	 <p>J5317.0510 J5317.0501 J5317.0502</p>	
 <p>Esthomic® Abutment, straight Esthomic® Abutment, angled 15°/20° Esthomic® Abutment, Inset</p>	 <p>J5317.0504 J5317.0503</p>	
 <p>Universal abutment Telescope abutment Gold-plastic abutment</p>		20 Ncm*
 <p>Logfit® Abutments Titanium bases CAD/CAM, crown and bridge</p>		
 <p>CONELOG® CAM titanium blank, type IAC and ME</p>		

* with the torque wrench J5320.1030

** Optional for temporary abutments titanium: torque after completed healing phase 20 Ncm.

All screws must be retightened with the corresponding torque after at least 5 minutes!

		3.3 mm	3.8 mm	4.3 mm	Ø 5.0 mm	3.3	3.8	4.3	5.0	6.0	
Article		Instrument				Tightening torque					
	Bar abutment, straight					20 Ncm*	30 Ncm*				
		J5300.0020	J5300.0021	J5300.0025							
	Bar abutment, 17° and 30° angled					20 Ncm*					
	Scanning cap for bar abutments					tightened by hand					
	Titanium cap for bar abutment, for crown/bridge					15 Ncm*					
	Crown base for bar abutment, burn-out										
		J5317.0510	J5317.0501	J5317.0502							
	Bases for bar abutments burn-out, cast-on, solderable, laser-weldable										
	Titanium bonding bases for bar abutment, Passive-Fit										
	Locator R-Tx® Abutment					20 Ncm*	30 Ncm*				
	Healing cap for bar abutment					tightened by hand					
	Impression cap for bar abutment, closed tray (bridge/bar)										
		J5300.0027	J5300.0028								
	Ball abutments					20 Ncm*	30 Ncm*				
		J5300.0011									
	Locator® Abutments					20 Ncm*					
	Locator® Fixture for bar abutment	J2253.0001									
	Scanbodies					tightened by hand					
	ScanPosts for Sirona® Scanbody										
		J5317.0501	J5317.0502								

* with the torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

Materials

Titanium Grade 4	
Properties (ASTM F67)	
Chemical structure (in %)	O ≤ 0.4
	Fe ≤ 0.5
	C ≤ 0.08
	N ≤ 0.05
	H ≤ 0.015
	Ti Rest
Mechanical properties	Tensile strength ≥ 550 MPa
	Elongation at break ≥ 12 %

Titanium alloy Ti6Al4V ELI	
Properties (ASTM F136)	
Chemical structure (in %)	Al 5.5 – 6.5
	V 3.5 – 4.5
	Fe ≤ 0.25
	C ≤ 0.08
	N ≤ 0.05
	O ≤ 0.13
	H ≤ 0.012
	Ti Rest
Mechanical properties	Tensile strength ≥ 860 MPa
	Elongation at break ≥ 10 %

Cast-on gold alloy CONELOG® Gold-plastic abutment	
Properties	
Chemical structure (in %)	Au 60
	Pd 20
	Pt 19
	Ir 1
Physical properties	Melting range 1400 – 1490 °C
	Density 17.5 g/cm ³
	E-Modul 136 GPa
	Coefficient of thermal expansion (25 – 500°C) 11.9 µm/m· °C
	Coefficient of thermal expansion (25 – 600°C) 12.2 µm/m· °C
	Color white
Mechanical properties	drawn
	Hardness HV5 > 215
	Tensile strength (Rm) > 750 MPa
	0.2% Elongation limit (Rp 0.2%) > 650 MPa
	Elongation at break > 2 %

Cast-on gold alloy base for bar abutment	
Properties	
Chemical structure (in %)	Au 60
	Pt 19
	Pd 20
	Ir 1
Physical properties	Density 17.5 g/cm ³
	Color white
	Liquidus 1490 °C
	Solidus 1400 °C
	Coefficient of thermal expansion (25 – 500°C) 12.5 µm/m· °C
	Coefficient of thermal expansion (25 – 600°C) 12.6 µm/m· °C
	E-Modul 136 GPa
Mechanical properties	hardened 700 °C/30 min.
	Hardness HV5 210
	0.2 % Elongation limit 450 – 570 MPa
	Elongation at break min. 10 %
	Tensile strength MPa 530 – 650

Solderable gold alloy base for bar abutment

Properties

Chemical structure (in %)	Au	68.60
	Pt	2.45
	Ag	11.85
	Pd	3.95
	Cu	10.60
	Zn	2.50
	Ir	0.05
	Rh	-
	Ru	-
Physical properties	Color	yellow
	Melting range	880 - 940 °C
Mechanical properties	Hardness	
	annealed HV5	175
	hardened HV5	275
	self hardened HV5	240

A		C	
Abutment collets	82	CAM titanium blank	64
Abutment screw for CONELOG® Titanium bases CAD/CAM	63	Cardanic driver	46
Abutment screw, hex	70, 77	Cleaning cannula	48
Adapter for screw implants	47	Cleaning needle	48
Adapter ISO shaft for angled hand piece	46	Collet for CAM blank, type IAC	64
Aligning tool	68	COMFOUR® Patient brochure	88
ALTApin applicator	53	Countersink	43
ALTApin magazine	55	Crown base for bar abutment	69
ALTApin membrane fixator	54	CT-tube	17
ALTApin pricker	54	D	
ALTApin pricker, insert	54	Demonstration model, acrylic glass	87
ALTApin set	53	Dense bone drill PROGRESSIVE-LINE	23
ALTApin single patient drill, ISO shaft	54	Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE	23, 37
ALTApin surgery mallet	54	Depth stop SCREW-LINE	43
ALTApin tray	53	DIM Analog® for the CONELOG® Implant System	59
Appointment pad	89	Disconnecter	81
B		Drill extension ISO shaft, for instruments with internal irrigation not for instruments with internal irrigation	41 44
Ball abutment analogs	72	Drill for CT-tube	17
Ball abutments, male part	71	Drill PROGRESSIVE-LINE Flex	27
Bar abutment	67	Driver for ball abutment	78
Bar implant analog for bar abutments	68	Driver for impression cap and healing cap for bar abutment	68, 79
Bar lab analog for bar abutments	68	Driver for Locator®	79
Bar sleeve for titanium bonding base	69	Driver for screw implants	45
Baring drill for cover screw	43	Driver for straight bar abutment	78, 79
Base for bar abutment	69	E	
Bite registration caps	59	Edentulous mandible	87
Bite registration posts	59		
Bone profiler	43		

E		G	
Esthomic® Abutments	60, 61	Guide System surgery set, SCREW-LINE	39
Esthomic® Abutments, Inset	61	Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30
Esthomic® Selection abutments	83	Guide System template drill	40
F		Guide System template drill PROGRESSIVE-LINE	32
Form drill PROGRESSIVE-LINE	23	Guiding pin for bone profiler	43
Form drill SCREW-LINE	37	H	
Form drill SCREW-LINE Cortical bone	37	Handle for CAMLOG®/CONELOG® Implant analog	81
G		Healing cap for bar abutment	68
Gingiva height indicator, straight	68	Healing cap	55
Gold-plastic abutment	65	Holding key for insertion post	47
Guide System check-up pin	41	Holding sleeve for screw implants	47
Guide System check-up pin PROGRESSIVE-LINE	32	I	
Guide System dense bone drill PROGRESSIVE-LINE	31	Implant analog	59
Guide System driver	41	Implant cover screw	55
Guide System form drill PROGRESSIVE-LINE	31	Implant pass	88
Guide System form drill	31	Impression cap for bar abutment, closed tray	68
for Ø 3.8 mm under preparation PROGRESSIVE-LINE		Impression caps for impression post, closed tray	58
Guide System form drill SCREW-LINE, Cortical bone	39	Impression posts	58
Guide System gingiva punch	39	L	
Guide System gingiva punch PROGRESSIVE-LINE	30	Lab analog	59
Guide System guiding sleeve	40	Lab prosthetic screw for bar abutment, hex	70
Guide System guiding sleeve PROGRESSIVE-LINE	32	Lab screw for CONELOG® Titanium bases CAD/CAM	63
Guide System Insertion post, screw-mounted	32, 40	Lab screw, hex	70, 77
Guide System pilot drill PROGRESSIVE-LINE	30	Lamella retention insert	71
Guide System pilot drill set	38	Locator® Abutment	74
Guide System pre-drill PROGRESSIVE-LINE	31	Locator® Abutment holder sleeve	79
Guide System seating tool	40		
Guide System setting tool PROGRESSIVE-LINE	32		

P		T	
PROGRESSIVE-LINE Implant, Promote® plus	19	Tap adapter	44
PROGRESSIVE-LINE Macro model	87	Tap PROGRESSIVE-LINE	23
Prosthetic screw for bar abutments	70	Tap SCREW-LINE	37
Prosthetic set	80	Telescope abutments, for double crown restorations	77
Prosthetic tray	80	Temporary abutment, titanium alloy	60
Prosthetic tray universal	80	Titanium bases CAD/CAM	62
R		Titanium bonding base for bar abutment	69
Removal adapter for CAMLOG® and CONELOG®	23	Titanium cap for bar abutment	68, 69
Reworking reamer, for base for bar abutment	82	Titanium cap without retention for bar abutment, for bridge	69
Round bur	42	Torque wrench	78
S		U	
Scanbodies	63	Universal abutments	65
Scanning cap for bar abutments	68	Universal abutments, for double crown restorations	77
ScanPosts for Sirona® Scanbody	63	Universal holder	82
Screw, hex	70	W	
Screwdriver Activator	78	Wrench adapter	27
Screwdriver, hex	47, 48, 80, 81	X	
SCREW-LINE Implant for practice	86	X-Ray Planning foil 1.25:1 CONELOG® PROGRESSIVE-LINE Implants	16
SCREW-LINE Implant, Promote® plus	33	CONELOG® SCREW-LINE Implants	16
SCREW-LINE Macro model	87	X-Ray Planning foil 1.4:1 CONELOG® PROGRESSIVE-LINE Implants	16
Selection abutment kit	83	CONELOG® SCREW-LINE Implants	16
Surgery set		X-Ray Transfer pictures 1.25:1 CONELOG® SCREW-LINE Implants	16
CAMLOG®/CONELOG® PROGRESSIVE-LINE	22		
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	26		
CAMLOG®/CONELOG® SCREW-LINE	36		
Surgery tray			
CAMLOG®/CONELOG® PROGRESSIVE-LINE	22		
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	26		
CAMLOG®/CONELOG® SCREW-LINE	36		
Surgery wash tray			
CAMLOG®/CONELOG® PROGRESSIVE-LINE	22		
CAMLOG®/CONELOG® SCREW-LINE	36		

Index Article number

05003503	Matrix CM Dalbo®-Plus	71	B1012	Point drill	42
05003504	Lamella retention insert	71		SCREW-LINE Implant, Promote® plus incl. screw-mounted insertion post	
07000389	Screwdriver Activator	78	C1065.3309	Ø 3.3 mm, L 9 mm	33
			C1065.3311	Ø 3.3 mm, L 11 mm	33
08394	Locator® Abutment holder sleeve	79	C1065.3313	Ø 3.3 mm, L 13 mm	33
			C1065.3316	Ø 3.3 mm, L 16 mm	33
	Locator® R-Tx™ Retention insert		C1065.3807	Ø 3.8 mm, L 7 mm	33
30001-01	Ø 3.3/3.8/4.3/5.0 mm, gray	73	C1065.3809	Ø 3.8 mm, L 9 mm	33
30002-01	Ø 3.3/3.8/4.3/5.0 mm, blue	73	C1065.3811	Ø 3.8 mm, L 11 mm	33
30003-01	Ø 3.3/3.8/4.3/5.0 mm, pink	73	C1065.3813	Ø 3.8 mm, L 13 mm	33
30004-01	Ø 3.3/3.8/4.3/5.0 mm, white	74	C1065.3816	Ø 3.8 mm, L 16 mm	33
			C1065.4307	Ø 4.3 mm, L 7 mm	33
	Locator® R-Tx™ Processing insert		C1065.4309	Ø 4.3 mm, L 9 mm	33
30012-01	Ø 3.3/3.8/4.3/5.0 mm	73	C1065.4311	Ø 4.3 mm, L 11 mm	33
			C1065.4313	Ø 4.3 mm, L 13 mm	33
	Locator® R-Tx™ Titanium housing		C1065.4316	Ø 4.3 mm, L 16 mm	33
30013-01	Ø 3.3/3.8/4.3/5.0 mm	73	C1065.5007	Ø 5.0 mm, L 7 mm	33
			C1065.5009	Ø 5.0 mm, L 9 mm	33
	Locator® R-Tx™ Analog		C1065.5011	Ø 5.0 mm, L 11 mm	33
30014-01	Ø 3.3/3.8/4.3 mm	72	C1065.5013	Ø 5.0 mm, L 13 mm	33
30016-01	Ø 5.0 mm	73	C1065.5016	Ø 5.0 mm, L 16 mm	33
				SCREW-LINE Implant, Promote® plus incl. snap-in insertion post	
30017-01	Locator® R-Tx™ Impression coping Ø 3.3/3.8/4.3/5.0 mm	72	C1066.3309	Ø 3.3 mm, L 9 mm	33
			C1066.3311	Ø 3.3 mm, L 11 mm	33
30018-01	Locator® R-Tx™ Processing spacer Ø 3.3/3.8/4.3/5.0 mm	73	C1066.3313	Ø 3.3 mm, L 13 mm	33
			C1066.3316	Ø 3.3 mm, L 16 mm	33
30021-01	Locator® R-Tx™ Retention insert tool	80	C1066.3807	Ø 3.8 mm, L 7 mm	33
			C1066.3809	Ø 3.8 mm, L 9 mm	33
	Locator® R-Tx™ Abutment		C1066.3811	Ø 3.8 mm, L 11 mm	33
30805-01	Ø 3.3 mm, GH 1.0 mm	72	C1066.3813	Ø 3.8 mm, L 13 mm	33
30805-02	Ø 3.3 mm, GH 2.0 mm	72	C1066.3816	Ø 3.8 mm, L 16 mm	33
30805-03	Ø 3.3 mm, GH 3.0 mm	72	C1066.4307	Ø 4.3 mm, L 7 mm	33
30805-04	Ø 3.3 mm, GH 4.0 mm	72	C1066.4309	Ø 4.3 mm, L 9 mm	33
30806-01	Ø 3.8 mm, GH 1.0 mm	72	C1066.4311	Ø 4.3 mm, L 11 mm	33
30806-02	Ø 3.8 mm, GH 2.0 mm	72	C1066.4313	Ø 4.3 mm, L 13 mm	33
30806-03	Ø 3.8 mm, GH 3.0 mm	72	C1066.4316	Ø 4.3 mm, L 16 mm	33
30806-04	Ø 3.8 mm, GH 4.0 mm	72	C1066.5007	Ø 5.0 mm, L 7 mm	33
30806-05	Ø 3.8 mm, GH 5.0 mm	72	C1066.5009	Ø 5.0 mm, L 9 mm	33
30807-01	Ø 4.3 mm, GH 1.0 mm	72	C1066.5011	Ø 5.0 mm, L 11 mm	33
30807-02	Ø 4.3 mm, GH 2.0 mm	72	C1066.5013	Ø 5.0 mm, L 13 mm	33
30807-03	Ø 4.3 mm, GH 3.0 mm	72	C1066.5016	Ø 5.0 mm, L 16 mm	33
30807-04	Ø 4.3 mm, GH 4.0 mm	72			
30807-05	Ø 4.3 mm, GH 5.0 mm	72			
30808-01	Ø 5.0 mm, GH 1.0 mm	72	C1069.3813	Ø 3.8 mm	86
30808-02	Ø 5.0 mm, GH 2.0 mm	72	C1069.4313	Ø 4.3 mm	86
30808-03	Ø 5.0 mm, GH 3.0 mm	72			
30808-04	Ø 5.0 mm, GH 4.0 mm	72			
30808-05	Ø 5.0 mm, GH 5.0 mm	72			
				SCREW-LINE Implant for practice	
				PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post	
A2002.2000	CT-tube	17	C1085.3309	Ø 3.3 mm, L 9 mm	19
			C1085.3311	Ø 3.3 mm, L 11 mm	19
			C1085.3313	Ø 3.3 mm, L 13 mm	19
	Drill for CT-tube		C1085.3316	Ø 3.3 mm, L 16 mm	19
A2050.2600	Ø 2.6 mm	17	C1085.3807	Ø 3.8 mm, L 7 mm	19
A2050.2800	Ø 2.8 mm	17	C1085.3809	Ø 3.8 mm, L 9 mm	19
			C1085.3811	Ø 3.8 mm, L 11 mm	19
A2222.2200	CT-tube	17	C1085.3813	Ø 3.8 mm, L 13 mm	19

	PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post			Healing cap, cylindrical	
C1085.3816	Ø 3.8 mm, L 16 mm	19	C2015.3820	Ø 3.8 mm, GH 2.0 mm	55
C1085.4307	Ø 4.3 mm, L 7 mm	19	C2015.3840	Ø 3.8 mm, GH 4.0 mm	55
C1085.4309	Ø 4.3 mm, L 9 mm	19	C2015.3860	Ø 3.8 mm, GH 6.0 mm	55
C1085.4311	Ø 4.3 mm, L 11 mm	19	C2015.4320	Ø 4.3 mm, GH 2.0 mm	55
C1085.4313	Ø 4.3 mm, L 13 mm	19	C2015.4340	Ø 4.3 mm, GH 4.0 mm	55
C1085.4316	Ø 4.3 mm, L 16 mm	19	C2015.4360	Ø 4.3 mm, GH 6.0 mm	55
C1085.5007	Ø 5.0 mm, L 7 mm	19	C2015.5020	Ø 5.0 mm, GH 2.0 mm	55
C1085.5009	Ø 5.0 mm, L 9 mm	19	C2015.5040	Ø 5.0 mm, GH 4.0 mm	55
C1085.5011	Ø 5.0 mm, L 11 mm	19	C2015.5060	Ø 5.0 mm, GH 6.0 mm	55
C1085.5013	Ø 5.0 mm, L 13 mm	19		Implant cover screw	
C1085.5016	Ø 5.0 mm, L 16 mm	19	C2019.3300	Ø 3.3 mm	55
	PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post		C2019.3800	Ø 3.8 mm	55
C1086.3309	Ø 3.3 mm, L 9 mm	19	C2019.4300	Ø 4.3 mm	55
C1086.3311	Ø 3.3 mm, L 11 mm	19	C2019.5000	Ø 5.0 mm	55
C1086.3313	Ø 3.3 mm, L 13 mm	19		Guide System CONELOG® Insertion post	
C1086.3316	Ø 3.3 mm, L 16 mm	19	C2026.3303	Ø 3.3 mm	32, 40
C1086.3807	Ø 3.8 mm, L 7 mm	19	C2026.3803	Ø 3.8 mm	32, 40
C1086.3809	Ø 3.8 mm, L 9 mm	19	C2026.4303	Ø 4.3 mm	32, 40
C1086.3811	Ø 3.8 mm, L 11 mm	19	C2026.5003	Ø 5.0 mm	32
C1086.3813	Ø 3.8 mm, L 13 mm	19		Impression post, closed tray	
C1086.3816	Ø 3.8 mm, L 16 mm	19	C2110.3300	Ø 3.3 mm	58
C1086.4307	Ø 4.3 mm, L 7 mm	19	C2110.3800	Ø 3.8 mm	58
C1086.4309	Ø 4.3 mm, L 9 mm	19	C2110.4300	Ø 4.3 mm	58
C1086.4311	Ø 4.3 mm, L 11 mm	19	C2110.5000	Ø 5.0 mm	58
C1086.4313	Ø 4.3 mm, L 13 mm	19		Impression post, open tray	
C1086.4316	Ø 4.3 mm, L 16 mm	19	C2121.3300	Ø 3.3 mm	58
C1086.5007	Ø 5.0 mm, L 7 mm	19	C2121.3800	Ø 3.8 mm	58
C1086.5009	Ø 5.0 mm, L 9 mm	19	C2121.4300	Ø 4.3 mm	58
C1086.5011	Ø 5.0 mm, L 11 mm	19	C2121.5000	Ø 5.0 mm	58
C1086.5013	Ø 5.0 mm, L 13 mm	19		Bite registration posts	
C1086.5016	Ø 5.0 mm, L 16 mm	19	C2140.3300	Ø 3.3 mm	59
	PROGRESSIVE-LINE Implant for practice		C2140.3800	Ø 3.8 mm	59
C1901.3813	Ø 3.8 mm	86	C2140.4300	Ø 4.3 mm	59
C1901.4313	Ø 4.3 mm	86	C2140.5000	Ø 5.0 mm	59
	Healing cap, bottleneck			Universal abutments	
C2011.3340	Ø 3.3 mm, GH 4.0 mm	55	C2211.3300	Ø 3.3 mm	65
C2011.3840	Ø 3.8 mm, GH 4.0 mm	55	C2211.3800	Ø 3.8 mm	65, 77
C2011.3860	Ø 3.8 mm, GH 6.0 mm	55	C2211.4300	Ø 4.3 mm	65, 77
C2011.4340	Ø 4.3 mm, GH 4.0 mm	55	C2211.5000	Ø 5.0 mm	65, 77
C2011.4360	Ø 4.3 mm, GH 6.0 mm	55		Telescope abutment for double crown restorations	
C2011.5040	Ø 5.0 mm, GH 4.0 mm	55	C2212.3800	Ø 3.8 mm	77
C2011.5060	Ø 5.0 mm, GH 6.0 mm	55	C2212.4300	Ø 4.3 mm	77
	Healing cap, wide body		C2212.5000	Ø 5.0 mm	77
C2014.3340	Ø 3.3 mm, GH 4.0 mm	55		Esthomic® Abutments, straight	
C2014.3840	Ø 3.8 mm, GH 4.0 mm	55	C2226.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	60
C2014.3860	Ø 3.8 mm, GH 6.0 mm	55	C2226.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	60
C2014.4340	Ø 4.3 mm, GH 4.0 mm	55	C2226.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	60
C2014.4360	Ø 4.3 mm, GH 6.0 mm	55	C2226.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	60
C2014.5040	Ø 5.0 mm, GH 4.0 mm	55	C2226.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	60
C2014.5060	Ø 5.0 mm, GH 6.0 mm	55	C2226.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	60
	Healing cap, cylindrical				
C2015.3320	Ø 3.3 mm, GH 2.0 mm	55			
C2015.3340	Ø 3.3 mm, GH 4.0 mm	55			

	Esthomic® Abutments, 15° angled, type A			Titanium bases CAD/CAM, crown	
C2227.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	60	C2242.3820	Ø 3.8 mm, GH 2.0 mm	62
C2227.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	60	C2242.4308	Ø 4.3 mm, GH 0.8 mm	62
C2227.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	60	C2242.4320	Ø 4.3 mm, GH 2.0 mm	62
C2227.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	60	C2242.5008	Ø 5.0 mm, GH 0.8 mm	62
C2227.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	60	C2242.5020	Ø 5.0 mm, GH 2.0 mm	62
C2227.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	60		Gold-plastic abutment	
	Esthomic® Abutments, 15° angled, type B		C2246.3300	Ø 3.3 mm	65
C2228.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	61	C2246.3800	Ø 3.8 mm	65
C2228.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	61	C2246.4300	Ø 4.3 mm	65
C2228.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	61	C2246.5000	Ø 5.0 mm	65
C2228.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	61		Ball abutments, male part	
C2228.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	61	C2249.3315	Ø 3.3 mm, GH 1.5 mm	71
C2228.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	61	C2249.3330	Ø 3.3 mm, GH 3.0 mm	71
	Esthomic® Abutments, 20° angled, type A		C2249.3815	Ø 3.8 mm, GH 1.5 mm	71
C2231.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	61	C2249.3830	Ø 3.8 mm, GH 3.0 mm	71
C2231.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	61	C2249.3845	Ø 3.8 mm, GH 4.5 mm	71
C2231.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	61	C2249.4315	Ø 4.3 mm, GH 1.5 mm	71
C2231.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	61	C2249.4330	Ø 4.3 mm, GH 3.0 mm	71
C2231.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	61	C2249.4345	Ø 4.3 mm, GH 4.5 mm	71
C2231.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	61	C2249.5015	Ø 5.0 mm, GH 1.5 mm	71
	Esthomic® Abutments, 20° angled, type B		C2249.5030	Ø 5.0 mm, GH 3.0 mm	71
C2232.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	61	C2249.5045	Ø 5.0 mm, GH 4.5 mm	71
C2232.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	61		Locator® Abutments	
C2232.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	61	C2253.3310	Ø 3.3 mm, GH 1.0 mm	74
C2232.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	61	C2253.3320	Ø 3.3 mm, GH 2.0 mm	74
C2232.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	61	C2253.3330	Ø 3.3 mm, GH 3.0 mm	74
C2232.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	61	C2253.3340	Ø 3.3 mm, GH 4.0 mm	74
	Esthomic® Abutments, Inset		C2253.3810	Ø 3.8 mm, GH 1.0 mm	74
C2235.3320	Ø 3.3 mm, GH 2.0 – 3.3 mm	61	C2253.3820	Ø 3.8 mm, GH 2.0 mm	74
C2235.3820	Ø 3.8 mm, GH 2.0 – 3.3 mm	61	C2253.3830	Ø 3.8 mm, GH 3.0 mm	74
C2235.4320	Ø 4.3 mm, GH 2.0 – 3.3 mm	61	C2253.3840	Ø 3.8 mm, GH 4.0 mm	74
C2235.5020	Ø 5.0 mm, GH 2.0 – 3.3 mm	61	C2253.3850	Ø 3.8 mm, GH 5.0 mm	74
	Temporary abutment, crown		C2253.4310	Ø 4.3 mm, GH 1.0 mm	74
C2239.3300	Ø 3.3 mm	60	C2253.4320	Ø 4.3 mm, GH 2.0 mm	74
C2239.3800	Ø 3.8 mm	60	C2253.4330	Ø 4.3 mm, GH 3.0 mm	74
C2239.4300	Ø 4.3 mm	60	C2253.4340	Ø 4.3 mm, GH 4.0 mm	74
C2239.5000	Ø 5.0 mm	60	C2253.4350	Ø 4.3 mm, GH 5.0 mm	74
	Modeling aids for CONELOG® Titanium bases CAD/CAM		C2253.5010	Ø 5.0 mm, GH 1.0 mm	74
C2242.3302	Ø 3.3 mm	63	C2253.5020	Ø 5.0 mm, GH 2.0 mm	74
C2242.3802	Ø 3.8 mm	63	C2253.5030	Ø 5.0 mm, GH 3.0 mm	74
C2242.4302	Ø 4.3 mm	63	C2253.5040	Ø 5.0 mm, GH 4.0 mm	74
C2242.5002	Ø 5.0 mm	63	C2253.5050	Ø 5.0 mm, GH 5.0 mm	74
	Titanium bases CAD/CAM, crown			Bar abutments, straight	
C2242.3308	Ø 3.3 mm, GH 0.8 mm	62	C2254.3310	Ø 3.3 mm, GH 1.0 mm	67
C2242.3320	Ø 3.3 mm, GH 2.0 mm	62	C2254.3325	Ø 3.3 mm, GH 2.5 mm	67
C2242.3808	Ø 3.8 mm, GH 0.8 mm	62	C2254.3810	Ø 3.8 mm, GH 1.0 mm	67
			C2254.3825	Ø 3.8 mm, GH 2.5 mm	67
			C2254.3840	Ø 3.8 mm, GH 4.0 mm	67
			C2254.4310	Ø 4.3 mm, GH 1.0 mm	67
			C2254.4325	Ø 4.3 mm, GH 2.5 mm	67
			C2254.4340	Ø 4.3 mm, GH 4.0 mm	67
			C2254.5010	Ø 5.0 mm, GH 1.0 mm	67
			C2254.5025	Ø 5.0 mm, GH 2.5 mm	67
			C2254.5040	Ø 5.0 mm, GH 4.0 mm	67

	Bar abutments, 17° angled, type A			CAM titanium blank, type ME	
C2256.3325	Ø 3.3 mm, GH 2.5 mm	67	C2421.3320	Ø 3.3 mm	64
C2256.3340	Ø 3.3 mm, GH 4.0 mm	67	C2421.3820	Ø 3.8 mm	64
C2256.3825	Ø 3.8 mm, GH 2.5 mm	67	C2421.4320	Ø 4.3 mm	64
C2256.3840	Ø 3.8 mm, GH 4.0 mm	67	C2421.5020	Ø 5.0 mm	64
C2256.4325	Ø 4.3 mm, GH 2.5 mm	67			
C2256.4340	Ø 4.3 mm, GH 4.0 mm	67		Logfit® Abutments	
C2256.5025	Ø 5.0 mm, GH 2.5 mm	67	C2550.3810	Ø 3.8 mm, GH 1.0 mm	66
C2256.5040	Ø 5.0 mm, GH 4.0 mm	67	C2550.3825	Ø 3.8 mm, GH 2.5 mm	66
			C2550.4310	Ø 4.3 mm, GH 1.0 mm	66
	Bar abutments, 17° angled, type B		C2550.4325	Ø 4.3 mm, GH 2.5 mm	66
C2257.3325	Ø 3.3 mm, GH 2.5 mm	67	C2550.5010	Ø 5.0 mm, GH 1.0 mm	66
C2257.3340	Ø 3.3 mm, GH 4.0 mm	67	C2550.5025	Ø 5.0 mm, GH 2.5 mm	66
C2257.3825	Ø 3.8 mm, GH 2.5 mm	67			
C2257.3840	Ø 3.8 mm, GH 4.0 mm	67		Scanbodies	
C2257.4325	Ø 4.3 mm, GH 2.5 mm	67	C2600.3310	Ø 3.3 mm	63
C2257.4340	Ø 4.3 mm, GH 4.0 mm	67	C2600.4310	Ø 3.8/4.3 mm	63
C2257.5025	Ø 5.0 mm, GH 2.5 mm	67	C2600.5010	Ø 5.0 mm	63
C2257.5040	Ø 5.0 mm, GH 4.0 mm	67			
				ScanPosts for Sirona® Scanbody	
	Bar abutments, 30° angled, type A		C2620.3306	Ø 3.3 mm	63
C2258.3325	Ø 3.3 mm, GH 2.5 mm	67	C2620.3806	Ø 3.8 mm	63
C2258.3340	Ø 3.3 mm, GH 4.0 mm	67	C2620.4306	Ø 4.3 mm	63
C2258.3825	Ø 3.8 mm, GH 2.5 mm	67	C2620.5006	Ø 5.0 mm	63
C2258.3840	Ø 3.8 mm, GH 4.0 mm	67			
C2258.4325	Ø 4.3 mm, GH 2.5 mm	67		Lab analog	
C2258.4340	Ø 4.3 mm, GH 4.0 mm	67	C3010.3300	Ø 3.3 mm	59
C2258.5035	Ø 5.0 mm, GH 2.5 mm	67	C3010.3800	Ø 3.8 mm	59
C2258.5050	Ø 5.0 mm, GH 4.0 mm	67	C3010.4300	Ø 4.3 mm	59
			C3010.5000	Ø 5.0 mm	59
	Bar abutments, 30° angled, type B			DIM Analog® for the CAMLOG® Implant System	
C2259.3325	Ø 3.3 mm, GH 2.5 mm	67	C3012.3300	Ø 3.3 mm	59
C2259.3340	Ø 3.3 mm, GH 4.0 mm	67	C3012.4300	Ø 3.8/4.3 mm	59
C2259.3825	Ø 3.8 mm, GH 2.5 mm	67	C3012.5000	Ø 5.0 mm	59
C2259.3840	Ø 3.8 mm, GH 4.0 mm	67			
C2259.4325	Ø 4.3 mm, GH 2.5 mm	67		Ball abutment analogs	
C2259.4340	Ø 4.3 mm, GH 4.0 mm	67	C3015.3300	Ø 3.3/3.8/4.3 mm	72
C2259.5035	Ø 5.0 mm, GH 2.5 mm	67	C3015.5000	Ø 5.0 mm	72
C2259.5050	Ø 5.0 mm, GH 4.0 mm	67			
	Temporary abutment, bridge			Implant analog	
C2339.3300	Ø 3.3 mm	60	C3025.3300	Ø 3.3 mm	59
C2339.3800	Ø 3.8 mm	60	C3025.3800	Ø 3.8 mm	59
C2339.4300	Ø 4.3 mm	60	C3025.4300	Ø 4.3 mm	59
C2339.5000	Ø 5.0 mm	60	C3025.5000	Ø 5.0 mm	59
	Titanium bases CAD/CAM, bridge				
C2342.3308	Ø 3.3 mm, GH 0.8 mm	62	C3709.0010	Universal holder	82
C2342.3320	Ø 3.3 mm, GH 2.0 mm	62			
C2342.3808	Ø 3.8 mm, GH 0.8 mm	62		Abutment collets	
C2342.3820	Ø 3.8 mm, GH 2.0 mm	62	C3709.3300	Ø 3.3 mm	82
C2342.4308	Ø 4.3 mm, GH 0.8 mm	62	C3709.3800	Ø 3.8 mm	82
C2342.4320	Ø 4.3 mm, GH 2.0 mm	62	C3709.4300	Ø 4.3 mm	82
C2342.5008	Ø 5.0 mm, GH 0.8 mm	62	C3709.5000	Ø 5.0 mm	82
C2342.5020	Ø 5.0 mm, GH 2.0 mm	62			
				Collet for CAM blank, type IAC	
	CAM titanium blank, type IAC		C3720.3300	Ø 3.3 mm	64
C2411.3313	Ø 3.3 mm	64	C3720.4300	Ø 3.8/4.3 mm	64
C2411.4313	Ø 3.8/4.3 mm	64	C3720.5000	Ø 5.0 mm	64
C2411.5013	Ø 5.0 mm	64			

Index Article number

	Lab screw with reduced head, hex		C8010.1010	SCREW-LINE Macro model	87
C4004.1600	Ø 3.3/3.8/4.3 mm	70			
C4004.2000	Ø 5.0 mm	70	C8010.1400	PROGRESSIVE-LINE Macro model	87
	Abutment screw with reduced head, hex		C8011.1000	Selection abutment kit	83
C4004.1601	Ø 3.3/3.8/4.3 mm	70			
C4004.2001	Ø 5.0 mm	70		Demonstration model, acrylic glass	
	Abutment screw, hex		C8050.1040	Lower jaw	87
C4005.1601	Ø 3.3/3.8/4.3 mm	77	C8070.1020	Upper jaw	87
C4005.2001	Ø 5.0 mm	77		Healing cap for bar abutment	
	Lab screw, hex		J2029.4300	Ø 3.3/3.8/4.3 mm	68
C4006.1601	Ø 3.3/3.8/4.3 mm	77	J2029.6000	Ø 5.0 mm	68
C4006.2001	Ø 5.0 mm	77		Impression caps for impression post, closed tray	
	Abutment screw for CONELOG® Titanium bases CAD/CAM		J2111.3300	Ø 3.3 mm	58
C4015.1601	Ø 3.3/3.8/4.3 mm	63	J2111.3800	Ø 3.8 mm	58
C4015.2001	Ø 5.0 mm	63	J2111.4300	Ø 4.3 mm	58
	Lab screw for CONELOG® Titanium bases CAD/CAM		J2111.5000	Ø 5.0 mm	58
C4016.1601	Ø 3.3/3.8/4.3 mm	63	J2112.3300	Bite registration caps Ø 3.3 mm	59
C4016.2001	Ø 5.0 mm	63	J2112.3800	Ø 3.8 mm	59
	CONELOG® Guiding pin for bone profiler		J2112.4300	Ø 4.3 mm	59
C5002.3300	Ø 3.3 mm	43	J2112.5000	Ø 5.0 mm	59
C5002.3800	Ø 3.8 mm	43		Impression cap, for bar abutment, closed tray (bridge/bar)	
C5002.4300	Ø 4.3 mm	43	J2129.4300	Ø 3.3/3.8/4.3 mm, short	68
C5002.5000	Ø 5.0 mm	43	J2129.4310	Ø 3.3/3.8/4.3 mm, long	68
	Disconnecter		J2129.6000	Ø 5.0 mm, short	68
C5300.1601	Ø 3.3/3.8/4.3 mm, short	81	J2129.6010	Ø 5.0/6.0 mm, long	68
C5300.1603	Ø 3.3/3.8/4.3 mm, long	81	J2253.0001	Driver for Locator®	79
C5300.2001	Ø 5.0 mm, short	81	J2253.0002	Locator® Instrument	79
C5300.2003	Ø 5.0 mm, long	81	J2253.0003	Locator® Angle measurement guide	79
C5300.9010	X-Ray Planning foil 1.25:1	16	J2253.0004	Locator® Parallel post	79
C5300.9011	X-Ray Planning foil 1.4:1	16	J2253.0102	Locator® Male processing package	75
	CONELOG® SCREW-LINE Implants		J2253.0112	Locator® Male processing package for extended range	75
C5300.9014	X-Ray Planning foil 1.25:1	16	J2253.0200	Locator® Impression cap	74
C5300.9015	X-Ray Planning foil 1.4:1	16	J2253.0340	Locator® Analog	74
	CONELOG® PROGRESSIVE-LINE Implants		J2253.0401	Locator® Block out spacer	75
C5300.9080	Ø 3.3 mm	16	J2253.0402	Locator® Processing replacement male	75
C5300.9081	Ø 3.8 mm	16		Locator® Replacement male	
C5300.9082	Ø 4.3 mm	16	J2253.1002	blue	76
C5300.9083	Ø 5.0 mm	16	J2253.1003	pink	76
	Adapter for screw implants		J2253.1005	clear	75
C5302.3310	Ø 3.3 mm, long	47			
C5302.3311	Ø 3.3 mm, short	47			
C5302.4310	Ø 3.8/4.3 mm, long	47			
C5302.4311	Ø 3.8/4.3 mm, short	47			
C5302.5011	Ø 5.0 mm, short	47			

	Locator® Replacement male for extended range		J2552.4300	Logfit® Analog Ø 3.8/4.3 mm	66
J2253.2000	Ø 3.8/4.3/5.0 mm, gray	76	J2552.6000	Ø 5.0 mm	66
J2253.2002	Ø 3.8/4.3/5.0 mm, red	76			
J2253.2003	Ø 3.8/4.3/5.0 mm, orange	76		Logfit® Plastic copings	
J2253.2004	Ø 3.8/4.3/5.0 mm, green	76	J2553.4301	Ø 3.8/4.3 mm, for bridges	66
	Locator® Fixture for bar abutment		J2553.4302	Ø 3.8/4.3 mm, for crowns	66
J2253.4301	Ø 3.3/3.8/4.3 mm	70	J2553.6001	Ø 5.0 mm, for bridges	66
J2253.6001	Ø 5.0 mm	70	J2553.6002	Ø 5.0 mm, for crowns	66
	Crown base for bar abutment		J2610.4300	Scanning cap for bar abutments Ø 3.3/3.8/4.3 mm	68
J2256.4306	Ø 3.3/3.8/4.3 mm	69	J2610.6000	Ø 5.0 mm	68
J2256.6006	Ø 5.0 mm	69			
	Base for bar abutment, burn-out		J3020.4300	Bar lab analog for bar abutments Ø 3.3/3.8/4.3 mm	68
J2257.4301	Ø 3.3/3.8/4.3 mm	69	J3020.6000	Ø 5.0 mm	68
J2257.6001	Ø 5.0 mm	69			
	Base for bar abutment, solderable		J3021.4300	Polishing protection for caps and bases Ø 3.3/3.8/4.3 mm	69
J2258.4300	Ø 3.3/3.8/4.3 mm	69	J3021.6000	Ø 5.0 mm	69
J2258.6000	Ø 5.0 mm	69			
	Titanium cap for bar abutment		J3025.0010	Handle for CAMLOG®/CONELOG® Implant analog Ø 3.3/3.8/4.3 mm	81
J2259.4301	Ø 3.3/3.8/4.3 mm, for crown	68	J3025.0015	Ø 5.0 mm	81
J2259.4302	Ø 3.3/3.8/4.3 mm, for bridge	69			
J2259.6001	Ø 5.0 mm, for crown	68		Bar implant analog for bar abutments Ø 3.3/3.8/4.3 mm	68
J2259.6002	Ø 5.0 mm, for bridge	69	J3025.4300	Ø 5.0 mm	68
	Titanium cap without retention for bar abutment, for bridge		J3025.6000		
J2259.4322	Ø 3.3/3.8/4.3 mm	69		Gingiva height indicator, straight Ø 3.3 mm	68
J2259.6022	Ø 5.0 mm	69	J3550.3300	Ø 3.8 mm	68
	Titanium bonding base for bar abutment		J3550.3800	Ø 4.3 mm	68
J2260.4301	Ø 3.3/3.8/4.3 mm	69	J3550.4300	Ø 5.0 mm	68
J2260.6001	Ø 5.0 mm	69	J3550.5000		68
	Bar sleeve for titanium bonding base		J3551.0001	Orientation gauge for COMFOUR®	68
J2261.4301	Ø 3.3/3.8/4.3 mm	69	J3709.0015	Universal holder	82
J2261.6001	Ø 5.0 mm	69			
	Base for bar abutment, laser-weldable		J3711.0010	Reworking reamer, for base for bar abutment Ø 3.3/3.8/4.3 mm, plane surface	82
J2262.4300	Ø 3.3/3.8/4.3 mm	69	J3711.0015	Ø 5.0 mm, plane surface	82
J2262.6000	Ø 5.0 mm	69	J3711.0020	Ø 3.3/3.8/4.3 mm, screw seat	82
	Base for bar abutment, cast-on		J3711.0025	Ø 5.0 mm, screw seat	82
J2263.4300	Ø 3.3/3.8/4.3 mm	69			
J2263.6000	Ø 5.0 mm	69		Guide System seating tool Ø 3.3 mm	40
J2269.0003	Aligning tool 17°	68	J3716.3300	Ø 3.8/4.3 mm	40
J2269.0004	Aligning tool 30°	68	J3716.4300		
J2269.0005	Aligning tool 17°	68		Guide System setting tool PROGRESSIVE-LINE	
J2269.0006	Aligning tool 30°	68	J3717.3300	Ø 3.3 mm	32
	Logfit® Impression caps		J3717.4300	Ø 3.8/4.3 mm	32
J2551.4300	Ø 3.8/4.3 mm	66	J3717.5000	Ø 5.0 mm	32
J2551.6000	Ø 5.0 mm	66			
			J3733.3300	Guide System template drill Ø 3.3 mm	40
			J3733.4300	Ø 3.8/4.3 mm	40

	Guide System guiding sleeve			Baring drill for cover screw	
J3734.3303	Ø 3.3 mm	40	J5004.4300	Ø 4.3 mm	43
J3734.3803	Ø 3.8 mm	40	J5004.5000	Ø 5.0 mm	43
J3734.4303	Ø 4.3 mm	40			
	Guide System template drill		J5006.3346	Ø 3.3 mm, Ø 4.6 mm	43
	PROGRESSIVE-LINE		J5006.3852	Ø 3.8 mm, Ø 5.2 mm	43
J3753.3300	Ø 3.3 mm	32	J5006.4356	Ø 4.3 mm, Ø 5.6 mm	43
J3753.4300	Ø 3.8/4.3 mm	32	J5006.5063	Ø 5.0 mm, Ø 6.3 mm	43
J3753.5000	Ø 5.0 mm	32			
	Guide System guiding sleeve			Depth stop SCREW-LINE for pilot drill	
	PROGRESSIVE-LINE		J5015.0007	L 7 mm	43
J3754.3301	Ø 3.3 mm	32	J5015.0009	L 9 mm	43
J3754.3801	Ø 3.8 mm	32	J5015.0011	L 11 mm	43
J3754.4301	Ø 4.3 mm	32	J5015.0013	L 13 mm	43
J3754.5001	Ø 5.0 mm	32			
	Plastic screw for bar abutment			Depth stop for form drill	
J4009.1627	M 1.6	71	J5015.3300	Ø 3.3 mm	23, 37
J4009.2027	M 2.0	71	J5015.3800	Ø 3.8 mm	23, 37
	Prosthetic screw for bar abutments		J5015.4300	Ø 4.3 mm	23, 37
J4012.1601	Ø 3.3/3.8/4.3 mm	70	J5015.5000	Ø 5.0 mm	23, 37
J4012.2001	Ø 5.0 mm	70			
	Screw, hex			Guide System gingiva punch	
J4012.1610	L 10 mm, M 1.6	70	J5041.3303	Ø 3.3 mm, SCREW-LINE	39
J4012.1615	L 15 mm, M 1.6	70	J5041.3304	Ø 3.3 mm, PROGRESSIVE-LINE	30
J4012.1620	L 20 mm, M 1.6	70	J5041.3803	Ø 3.8 mm, SCREW-LINE	39
J4012.2010	L 10 mm, M 2.0	70	J5041.3804	Ø 3.8 mm, PROGRESSIVE-LINE	30
J4012.2015	L 15 mm, M 2.0	70	J5041.4303	Ø 4.3 mm, SCREW-LINE	39
J4012.2020	L 20 mm, M 2.0	70	J5041.4304	Ø 4.3 mm, PROGRESSIVE-LINE	30
	Lab prosthetic screw for bar abutment		J5041.5004	Ø 5.0 mm, PROGRESSIVE-LINE	30
J4013.1601	Ø 3.3/3.8/4.3 mm	70	J5050.2300	Round bur	42
J4013.2001	Ø 5.0 mm	70	J5051.2000	Pilot drill SCREW-LINE	42
	Drill extension ISO shaft		J5051.2003	Pilot drill	42
J5002.0005	for instruments with internal irrigation	41	J5051.2800	Pre-drill SCREW-LINE	42
J5002.0006	not for instruments with internal irrigation	44			
J5002.0011	Adapter ISO shaft	46	J5053.3316	Form drill SCREW-LINE Cortical bone	
J5002.0012	Cleaning needle	48	J5053.3816	Ø 3.3 mm	37
J5002.0013	Wrench adapter	27	J5053.4316	Ø 3.8 mm	37
J5002.0020	Cleaning cannula	48	J5053.5016	Ø 4.3 mm	37
	Bone profiler		J5054.3016	Ø 5.0 mm	37
J5003.3350	Ø 3.3 mm	43			
J5003.4360	Ø 3.8/4.3 mm	43	J5054.3309	Tap SCREW-LINE	
J5003.5070	Ø 5.0 mm	43	J5054.3809	Ø 3.3 mm	37
	Baring drill for cover screw		J5054.4309	Ø 3.8 mm	37
J5004.3300	Ø 3.3 mm	43	J5054.5009	Ø 4.3 mm	37
J5004.3800	Ø 3.8 mm	43	J5062.3309	Ø 5.0 mm	37
			J5062.3311	Form drill SCREW-LINE	
			J5062.3313	Ø 3.3 mm, L 9	37
			J5062.3316	Ø 3.3 mm, L 11	37
			J5062.3316	Ø 3.3 mm, L 13	37
			J5062.3316	Ø 3.3 mm, L 16	37
			J5062.3807	Ø 3.8 mm, L 7	37

	Form drill SCREW-LINE			Form drill PROGRESSIVE-LINE	
J5062.3809	Ø 3.8 mm, L 9	37	J5070.3309	Ø 3.3 mm, L 9 mm	23
J5062.3811	Ø 3.8 mm, L 11	37	J5070.3311	Ø 3.3 mm, L 11 mm	23
J5062.3813	Ø 3.8 mm, L 13	37	J5070.3313	Ø 3.3 mm, L 13 mm	23
J5062.3816	Ø 3.8 mm, L 16	37	J5070.3316	Ø 3.3 mm, L 16 mm	23
J5062.4307	Ø 4.3 mm, L 7	37	J5070.3807	Ø 3.8 mm, L 7 mm	23
J5062.4309	Ø 4.3 mm, L 9	37	J5070.3809	Ø 3.8 mm, L 9 mm	23
J5062.4311	Ø 4.3 mm, L 11	37	J5070.3811	Ø 3.8 mm, L 11 mm	23
J5062.4313	Ø 4.3 mm, L 13	37	J5070.3813	Ø 3.8 mm, L 13 mm	23
J5062.4316	Ø 4.3 mm, L 16	37	J5070.3816	Ø 3.8 mm, L 16 mm	23
J5062.5007	Ø 5.0 mm, L 7	37	J5070.4307	Ø 4.3 mm, L 7 mm	23
J5062.5009	Ø 5.0 mm, L 9	37	J5070.4309	Ø 4.3 mm, L 9 mm	23
J5062.5011	Ø 5.0 mm, L 11	37	J5070.4311	Ø 4.3 mm, L 11 mm	23
J5062.5013	Ø 5.0 mm, L 13	37	J5070.4313	Ø 4.3 mm, L 13 mm	23
J5062.5016	Ø 5.0 mm, L 16	37	J5070.4316	Ø 4.3 mm, L 16 mm	23
	Guide System pilot drill set		J5070.5007	Ø 5.0 mm, L 7 mm	23
J5063.3309	Ø 3.3 mm, L 5/9 mm	38	J5070.5009	Ø 5.0 mm, L 9 mm	23
J5063.3311	Ø 3.3 mm, L 5/9/11 mm	38	J5070.5011	Ø 5.0 mm, L 11 mm	23
J5063.3313	Ø 3.3 mm, L 5/9/13 mm	38	J5070.5013	Ø 5.0 mm, L 13 mm	23
J5063.4307	Ø 3.8/4.3 mm, L 5/7 mm	38	J5070.5016	Ø 5.0 mm, L 16 mm	23
J5063.4309	Ø 3.8/4.3 mm, L 5/9 mm	38		Tap PROGRESSIVE-LINE	
J5063.4311	Ø 3.8/4.3 mm, L 5/9/11 mm	38	J5071.3300	Ø 3.3 mm	23
J5063.4313	Ø 3.8/4.3 mm, L 5/9/11/13 mm	38	J5071.3800	Ø 3.8 mm	23
J5064.3316	Ø 3.3 mm, L 16 mm	38	J5071.4300	Ø 4.3 mm	23
J5064.4316	Ø 3.8/4.3 mm, L 16 mm	38	J5071.5000	Ø 5.0 mm	23
	Guide System surgery set, SCREW-LINE			Dense bone drill PROGRESSIVE-LINE	
J5065.3309	Ø 3.3 mm, L 5/9 mm	39	J5072.3300	Ø 3.3 mm	23
J5065.3311	Ø 3.3 mm, L 5/9/11 mm	39	J5072.3800	Ø 3.8 mm	23
J5065.3313	Ø 3.3 mm, L 5/9/11/13 mm	39	J5072.4300	Ø 4.3 mm	23
J5065.3807	Ø 3.8 mm, L 5/7 mm	39	J5072.5000	Ø 5.0 mm	23
J5065.3809	Ø 3.8 mm, L 5/9 mm	39		Guide System pilot drill PROGRESSIVE-LINE	
J5065.3811	Ø 3.8 mm, L 5/9/11 mm	39	J5074.3305	Ø 3.3 mm, L 5 mm	30
J5065.3813	Ø 3.8 mm, L 5/9/11/13 mm	39	J5074.3309	Ø 3.3 mm, L 9 mm	30
J5065.4307	Ø 4.3 mm, L 5/7 mm	39	J5074.3311	Ø 3.3 mm, L 11 mm	30
J5065.4309	Ø 4.3 mm, L 5/9 mm	39	J5074.3313	Ø 3.3 mm, L 13 mm	30
J5065.4311	Ø 4.3 mm, L 5/9/11 mm	39	J5074.3316	Ø 3.3 mm, L 16 mm	30
J5065.4313	Ø 4.3 mm, L 5/9/11/13 mm	39	J5074.4305	Ø 3.8/4.3 mm, L 5 mm	30
J5066.3316	Ø 3.3 mm, L 16 mm	39	J5074.4307	Ø 3.8/4.3 mm, L 7 mm	30
J5066.3816	Ø 3.8 mm, L 16 mm	39	J5074.4309	Ø 3.8/4.3 mm, L 9 mm	30
J5066.4316	Ø 4.3 mm, L 16 mm	39	J5074.4311	Ø 3.8/4.3 mm, L 11 mm	30
	Guide System form drill, SCREW-LINE, Cortical Bone		J5074.4313	Ø 3.8/4.3 mm, L 13 mm	30
J5068.3309	Ø 3.3 mm, L 9 mm	39	J5074.4316	Ø 3.8/4.3 mm, L 16 mm	30
J5068.3311	Ø 3.3 mm, L 11 mm	39	J5074.5005	Ø 5.0 mm, L 5 mm	30
J5068.3313	Ø 3.3 mm, L 13 mm	39	J5074.5007	Ø 5.0 mm, L 7 mm	30
J5068.3316	Ø 3.3 mm, L 16 mm	39	J5074.5009	Ø 5.0 mm, L 9 mm	30
J5068.3807	Ø 3.8 mm, L 7 mm	39	J5074.5011	Ø 5.0 mm, L 11 mm	30
J5068.3809	Ø 3.8 mm, L 9 mm	39	J5074.5013	Ø 5.0 mm, L 13 mm	30
J5068.3811	Ø 3.8 mm, L 11 mm	39	J5074.5016	Ø 5.0 mm, L 16 mm	30
J5068.3813	Ø 3.8 mm, L 13 mm	39		Guide System pre-drill PROGRESSIVE-LINE	
J5068.3816	Ø 3.8 mm, L 16 mm	39	J5076.3305	Ø 3.3 mm	31
J5068.4307	Ø 4.3 mm, L 7 mm	39	J5076.3805	Ø 3.8 mm	31
J5068.4309	Ø 4.3 mm, L 9 mm	39	J5076.4305	Ø 4.3 mm	31
J5068.4311	Ø 4.3 mm, L 11 mm	39	J5076.5005	Ø 5.0 mm	31
J5068.4313	Ø 4.3 mm, L 13 mm	39			
J5068.4316	Ø 4.3 mm, L 16 mm	39			

	Guide System form drill			Profile drill PROGRESSIVE-LINE Flex	
	PROGRESSIVE-LINE		J5080.4300	Ø 4.3 mm	27
J5076.3309	Ø 3.3 mm, L 9 mm	31	J5080.5000	Ø 5.0 mm	27
J5076.3311	Ø 3.3 mm, L 11 mm	31			
J5076.3313	Ø 3.3 mm, L 13 mm	31	J5300.0011	Driver	78
J5076.3316	Ø 3.3 mm, L 16 mm	31		for ball abutment, manual/wrench	
J5076.3807	Ø 3.8 mm, L 7 mm	31		Driver for straight bar abutment	
J5076.3809	Ø 3.8 mm, L 9 mm	31	J5300.0020	Ø 3.3/3.8/4.3 mm, short	78
J5076.3811	Ø 3.8 mm, L 11 mm	31	J5300.0021	Ø 3.3/3.8/4.3 mm, long	79
J5076.3813	Ø 3.8 mm, L 13 mm	31	J5300.0025	Ø 5.0 mm, short	78
J5076.3816	Ø 3.8 mm, L 16 mm	31		Removal adapter for	
J5076.4307	Ø 4.3 mm, L 7 mm	31		CAMLOG® and CONELOG®	
J5076.4309	Ø 4.3 mm, L 9 mm	31	J5300.0022	Ø 3.3/3.8/4.3/5.0 mm	23
J5076.4311	Ø 4.3 mm, L 11 mm	31		Driver for impression cap and	
J5076.4313	Ø 4.3 mm, L 13 mm	31		healing cap for bar abutment	
J5076.4316	Ø 4.3 mm, L 16 mm	31	J5300.0027	Ø 3.3/3.8/4.3 mm	68, 79
J5076.5007	Ø 5.0 mm, L 7 mm	31	J5300.0028	Ø 5.0 mm	68, 79
J5076.5009	Ø 5.0 mm, L 9 mm	31			
J5076.5011	Ø 5.0 mm, L 11 mm	31	J5300.0030	PickUp instrument	46
J5076.5013	Ø 5.0 mm, L 13 mm	31		Driver for screw implants	
J5076.5016	Ø 5.0 mm, L 16 mm	31	J5300.0031	extra short, manual/wrench	45
	Guide System form drill for Ø 3.8 mm		J5300.0032	short, manual/wrench	45
	under preparation PROGRESSIVE-LINE		J5300.0033	long, manual/wrench	45
J5077.3309	Ø 3.3 mm, L 9 mm	31		with ISO-shaft for angled hand piece	
J5077.3311	Ø 3.3 mm, L 11 mm	31	J5300.0034	short (with hexagon at the shaft)	45
J5077.3313	Ø 3.3 mm, L 13 mm	31	J5300.0035	long (with hexagon at the shaft)	45
J5077.3316	Ø 3.3 mm, L 16 mm	31	J5300.0036	short (without hexagon at the shaft)	46
	Guide System dense bone drill		J5300.0037	long (without hexagon at the shaft)	46
	PROGRESSIVE-LINE		J5300.0038	Cardanic driver	46
J5078.3309	Ø 3.3 mm, L 9 mm	31		Surgery set CAMLOG®/CONELOG®	
J5078.3311	Ø 3.3 mm, L 11 mm	31	J5300.0063	SCREW-LINE	36
J5078.3313	Ø 3.3 mm, L 13 mm	31	J5300.0065	PROGRESSIVE-LINE	22
J5078.3316	Ø 3.3 mm, L 16 mm	31	J5300.0071	PROGRESSIVE-LINE Flex	26
J5078.3807	Ø 3.8 mm, L 7 mm	31		Pattern for surgery wash tray	
J5078.3809	Ø 3.8 mm, L 9 mm	31		CAMLOG®/CONELOG®	
J5078.3811	Ø 3.8 mm, L 11 mm	31	J5300.1068	SCREW-LINE	36
J5078.3813	Ø 3.8 mm, L 13 mm	31	J5300.1070	PROGRESSIVE-LINE	22
J5078.3816	Ø 3.8 mm, L 16 mm	31		Paralleling pin	
J5078.4307	Ø 4.3 mm, L 7 mm	31	J5300.2000	PROGRESSIVE-LINE	23
J5078.4309	Ø 4.3 mm, L 9 mm	31	J5300.2028	SCREW-LINE	44
J5078.4311	Ø 4.3 mm, L 11 mm	31		Surgery tray (without content)	
J5078.4313	Ø 4.3 mm, L 13 mm	31		CAMLOG®/CONELOG®	
J5078.4316	Ø 4.3 mm, L 16 mm	31	J5300.8916	SCREW-LINE	36
J5078.5007	Ø 5.0 mm, L 7 mm	31	J5300.8917	PROGRESSIVE-LINE	22
J5078.5009	Ø 5.0 mm, L 9 mm	31	J5300.8920	PROGRESSIVE-LINE Flex	26
J5078.5011	Ø 5.0 mm, L 11 mm	31		Guide System surgery tray	
J5078.5013	Ø 5.0 mm, L 13 mm	31		CAMLOG®/CONELOG® (without content)	
J5078.5016	Ø 5.0 mm, L 16 mm	31	J5300.8919	PROGRESSIVE-LINE	30
	Drill PROGRESSIVE-LINE Flex				
J5079.3300	Ø 3.3 mm	27			
J5079.3800	Ø 3.8 mm	27			
J5079.4300	Ø 4.3 mm	27			
J5079.5000	Ø 5.0 mm	27			
	Profile drill PROGRESSIVE-LINE Flex				
J5080.3300	Ø 3.3 mm	27			
J5080.3800	Ø 3.8 mm	27			

	Surgery wash tray (without content) CAMLOG®/CONELOG®		J5418.5000	Osteotome SCREW-LINE Ø 5.0 mm, straight convex	49
J5300.8968	SCREW-LINE	36	J5418.5010	Ø 5.0 mm, angled convex	50
J5300.8970	PROGRESSIVE-LINE	22		Pre-Osteotome SCREW-LINE	
	Guide System check-up pin		J5419.2800	1.7 – 2.8 mm, straight concave	51, 52
J5301.3300	Ø 3.3 mm, SCREW-LINE	41		Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE,	
J5301.3310	Ø 3.3 mm, PROGRESSIVE-LINE	32		straight concave	51
J5301.4300	Ø 3.8/4.3 mm, SCREW-LINE	41	J5420.0020	angled concave	52
J5301.4310	Ø 3.8/4.3 mm, PROGRESSIVE-LINE	32	J5420.0030		
J5301.5010	Ø 5.0 mm, PROGRESSIVE-LINE	32		Osteotome SCREW-LINE	
J5302.0010	Holding key for insertion post	47	J5420.3300	Ø 3.3 mm, straight concave	51
	Holding sleeve for screw implants		J5420.3310	Ø 3.3 mm, angled concave	52
J5302.3300	Ø 3.3 mm	47	J5420.3800	Ø 3.8 mm, straight concave	51
J5302.3800	Ø 3.8 mm	47	J5420.3810	Ø 3.8 mm, angled concave	52
J5302.4300	Ø 4.3 mm	47	J5420.4300	Ø 4.3 mm, straight concave	51
J5302.5000	Ø 5.0 mm	47	J5420.4310	Ø 4.3 mm, angled concave	52
	Guide System driver		J5420.5000	Ø 5.0 mm, straight concave	51
J5303.4300	Ø 3.3/3.8/4.3 mm, manual/wrench	41	J5420.5010	Ø 5.0 mm, angled concave	52
J5304.4300	Ø 3.3/3.8/4.3 mm, with ISO shaft	41	J8070.2050	Edentulous mandible	87
	Screwdriver, hex		M1000.0050	ALTApin magazine, 1 unit	55
J5317.0501	short, manual/wrench	47, 80	M1000.0100	ALTApin magazine, 3 units	55
J5317.0502	long, manual/wrench	47, 81	M5100.0010	ALTApin applicator, straight	53
J5317.0503	long, ISO shaft	48, 81	M5100.0030	ALTApin applicator, angled 90°	53
J5317.0504	short, ISO shaft	48, 81	M5100.0050	ALTApin pricker	54
J5317.0510	extra short, manual/wrench	47, 80	M5100.0070	ALTApin membrane fixator	54
J5317.0511	Manual screwdriver, hex	48, 81	M5100.0100	ALTApin surgery mallet	54
J5320.1030	Torque wrench	78	M5200.0010	ALTApin applicator, straight, work element	53
	Tap adapter		M5200.0055	ALTApin pricker, insert	54
J5322.0010	short	44	M5500.0050	ALTApin single patient drill, ISO shaft	54
J5322.0011	long	44	M5600.0110	ALTApin set	53
J5330.8500	Prosthetic tray	80	M5600.0210	ALTApin tray	53
J5330.8600	Prosthetic set	80		Osteotomy set CAMLOG®/ CONELOG® SCREW-LINE,	
J5330.8700	Prosthetic tray universal	80		straight convex	49
	Pre-Osteotome SCREW-LINE			angled convex	50
J5417.2800	1.7 – 2.8 mm, straight convex	49, 50		Osteotome SCREW-LINE	
				Ø 3.3 mm, straight convex	49
J5418.0020				Ø 3.3 mm, angled convex	50
J5418.0030				Ø 3.8 mm, straight convex	49
				Ø 3.8 mm, angled convex	50
J5418.3300				Ø 4.3 mm, straight convex	49
J5418.3310				Ø 4.3 mm, angled convex	50
J5418.3800					
J5418.3810					
J5418.4300					
J5418.4310					

Further documentation

Further information on the CONELOG® Products can be found in the following documents:

- CONELOG® Product catalog
- CONELOG® Working instructions
- CONELOG® Instruction for use
- Preparation instructions
- Camlog literature overview
- Camlog and science

The documents are available from the local Camlog representative.

See also:

<https://ifu.camlog.com>

www.camlog.com

References

- [1] Conserva E. Initial stability after placement of a new buttress threaded implant. A case series study. implants. 2019(3): 24-28.
- [2] Ruppin J. One-year clinical experience with Progressive-Line implants. EDI journal. 2020(4): 54-63.
- [3] Semper-Hogg W, Kraft S, Stiller S, Mehrhof J, Nelson K. Analytical and experimental position stability of the abutment in different dental implant systems with a conical implant-abutment connection. Clin Oral Investig 2010;17(3): 1017-23.
- [4] Semper Hogg W, Zulauf K, Mehrhof J, Nelson K. The influence of torque tightening on the position stability of the abutment in conical implant-abutment connections. Int J Prosthodont 2015;28: 538-41.

Trademarks and copyright

Protected trade names (trademarks) are not always specially indicated. The absence of such an indication does not mean that this name is NOT a trademark. The document including all its parts is protected by copyright. You may download the content regarding the intended use, but changes to or reproduction of the content are not permitted. Any exploitation beyond the narrow limits of the copyright act is not permitted without prior written approval of CAMLOG Biotechnologies GmbH and is subject to legal sanctions.

CE0123

Art. No. J8001.0009 Rev.07 07/2021



Headquarters

CAMLOG Biotechnologies GmbH | Margarethenstr. 38 | 4053 Basel | Switzerland
Phone +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.camlog.com

Manufacturer CAMLOG® and CONELOG® Products: ALTATEC GmbH | Maybachstr. 5 | 71299 Wimsheim | Germany

